



INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification⁶ :

A61J 2/06

A2

(11) International Publication Number:

WO 98/23242

(43) International Publication Date:

4 June 1998 (04.06.98)

(21) International Application Number:

PCT/US97/21211

(22) International Filing Date:

13 November 1997 (13.11.97)

(30) Priority Data:

08/756,061


25 November 1996 (25.11.96) US

(71) Applicant: C.R. BARD, INC. [US/US]; 730 Central Avenue,
Murray Hill, NJ 07974 (US).(72) Inventors: ROBINSON, Timothy; 11 Snow Lane, Sandown,
NH 03873 (US). WEISER, Michael, F.; 516 Martins Pond
Road, Groton, MA 01450 (US). KUJAWSKI, Dennis;
25 Parker Road, Brookline, NH 03033 (US). DWYER,
Clifford, J.; 9 Moore Street, Wilmington, MA 01887 (US).(74) Agent: BOOKSTEIN, Arthur; One Beacon Street, Boston, MA
02108 (US).

(54) Title: MODULAR ENDOPROSTHESIS

(57) Abstract

An endoprosthetic implant is formed from a plurality of separate individual components that are inserted sequentially and transuminally into a bifurcated vascular region with each component being deployed in sequence by a sequence of catheter-like deployment devices. The separate components are placed relative to each other to define a bifurcated endoprosthesis. In one embodiment the deployment device includes a tubular sheath for maintaining the radially expandable tubular implant in a contracted configuration and a gripping device including a cup and a gripping member that cooperate to define an annular space by which the trailing end of the implant can be securely held by the deployment device during positioning of the device.

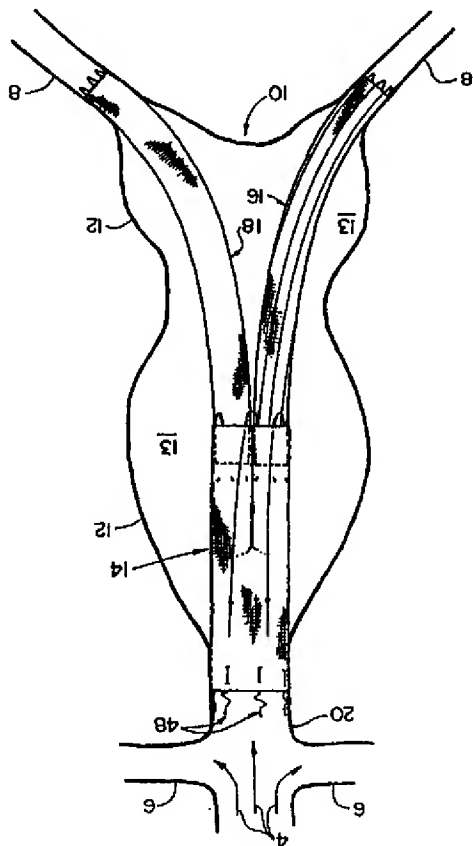

Published
Without international search report and to be republished
upon receipt of that report.

(81) Designated States: AU, CA, JP, European patent (AT, BE,
CH, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL,
PT, SE).

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

FOR THE PURPOSES OF INFORMATION ONLY

AL	Albania	ES	Spain	LS	Lesotho	SI	Slovenia
AM	Armenia	FI	Finland	LT	Lithuania	SK	Slovakia
AT	Austria	FR	France	LU	Luxembourg	SN	Senegal
AU	Australia	GA	Gabon	LV	Latvia	SZ	Swaziland
AZ	Azerbaijan	GB	United Kingdom	MC	Monaco	TD	Togo
BA	Bosnia and Herzegovina	GE	Georgia	MD	Republic of Moldova	TG	Togo
BB	Barbados	GH	Ghana	MG	Madagascar	TJ	Tajikistan
BE	Belgium	GN	Guinea	MK	The former Yugoslav	TM	Turkmenistan
BF	Burkina Faso	GR	Greece	ML	Mali	TR	Turkey
BG	Bulgaria	HU	Hungary	MN	Mongolia	TT	Trinidad and Tobago
BJ	Benin	IE	Ireland	MR	Mauritania	UA	Ukraine
BR	Brazil	IL	Israel	MW	Malawi	UG	Uganda
BY	Belarus	IS	Iceland	MX	Mexico	UZ	Uzbekistan
CA	Canada	IT	Italy	NE	Niger	VN	Viet Nam
CF	Central African Republic	JP	Japan	NL	Netherlands	YU	Yugoslavia
CG	Congo	KR	Korea	NO	Norway	ZW	Zimbabwe
CH	Switzerland	KG	Kyrgyzstan	NZ	New Zealand		
CI	Côte d'Ivoire	KP	Democratic People's	PL	Poland		
CM	Cameroon	KR	Republic of Korea	PT	Portugal		
CN	China	KZ	Kazakhstan	RO	Romania		
CU	Cuba	LC	Saint Lucia	RU	Russian Federation		
CZ	Czech Republic	LI	Liechtenstein	SD	Sudan		
DE	Germany	LK	Sri Lanka	SG	Singapore		
DK	Denmark	LR	Liberia				
EE	Estonia						

MODULAR ENDOPROSTHESIS

Field of the Invention

The invention relates to devices and techniques for placing and securing an endoprosthesis in a patient's vascular system, including bifurcated blood vessels.

5

Background of the Invention

Among the long accepted practices to treat a variety of vascular disorders are surgical procedures that involve placement of a tubular graft in a patient's blood vessels. The construction and characteristics of the graft typically are adapted to optimize its use in the specific surgical environment and condition to

10

be treated and, accordingly, a number of different types of grafts are available. Among the most common vascular grafts are those formed from a woven or knitted tubular fabric as well as non-fabric tubes such as expanded

polytetrafluoroethylene. Such grafts typically are placed in a patient's vascular system in a highly invasive surgical procedure. In general, the complexity of the surgical procedure required to place the graft will depend on many factors, including the location and surgical accessibility of the portion of the patient's vasculature where the graft is to be placed.

15

Not all vascular conditions in which it would be desirable to place a graft can be so treated. Among the particularly troublesome medical conditions in which it is desirable to place a graft is that of an abdominal aortic aneurysm, in

20

which a portion of the patient's aorta, the major artery carrying blood from the heart, has developed a weakened wall such that the weakened portion will tend to expand under the influence of the patient's blood pressure. An aortic

25

aneurysm presents a life threatening risk that the aneurysm may burst causing massive internal bleeding. Treatment of the condition typically has involved deeply invasive abdominal surgery in which the patient's abdominal cavity is

opened to reach and expose the aortic aneurysm. While maintaining the patient on an independent life support system, the region of the aneurysm is incised lengthwise to enable insertion of the graft into the aorta to span the weakened region and define a structurally strong tubular flow path between the remaining healthy portions of the aorta. The graft, so positioned, then is sutured in place. The graft thus serves as a reinforcing liner for the weakened portion of the aorta. Such surgical procedures have been characterized by a relatively high mortality rate. Typically, patients suffering from the condition are elderly and are less able to survive the rigors of major abdominal surgery. Additionally, there is a substantial degree of risk when the abdominal cavity is opened because the confining pressure of other abdominal organs on the aorta is released. In some cases, the aortic wall in the region of the aneurysm is so weak that upon release of the confining pressure, the aneurysm may burst with resulting immediate massive hemorrhaging.

Significant effort has been directed to the development of less invasive techniques for placement of a graft, such as in the abdominal aortic region, in a manner that presents less risk to the patient. Various devices in the form of a single tubular implant have been described for that purpose. Typically, such single tube devices have a means for anchoring the ends of the graft to healthy vascular tissue at the opposite ends of the aneurysmal region.

In the case of abdominal aortic aneurysms, however, by the time the aneurysm is discovered, it may have advanced to a stage where there is insufficient healthy tissue in the region where the aorta bifurcates into the two iliac arteries for the end of a single tubular graft to be secured. Often the aneurysm has advanced into and involves the iliac arteries as well. Such a condition cannot be treated by a single lumen tubular prosthesis. If an endoluminal prosthesis is to be placed in such anatomy, the prosthesis must have a bifurcated configuration in order to extend fully through the regions of aneurysm in all of the involved arteries and with the device being in secure

engagement with healthy tissue to insure that it provides full endoluminal support and will not migrate from its implanted position.

The necessity for the use of a bifurcated graft has been recognized. One approach is described in U.S. patent 5,489,295 (Piplani) in which a one-piece bifurcated graft is described as being placed in the bifurcated region of the aorta and iliac arteries. The procedure described is complex and requires many difficult manipulations by the physician. Additionally, the unpredictable variations and vascular anatomy of an individual patient can be expected to present blood vessels of shapes and diameters that do not readily match the preformed configuration of a one piece, preformed, bifurcated graft. Consequently, the use of such a graft is likely to result in mismatches between one or more of the three legs of the bifurcated graft with the corresponding aorta and iliac arteries.

Another device is described in PCT patent application PCT/US95/01466 (International Publication No. WO95/21592) in which a bifurcated device is formed in two sections, one of which includes a graft having a main body and one integral leg extension. The main body is intended to be placed in the aorta and the extension in one of iliac arteries. The main body also has an opening adjacent the leg extension that can be aligned with the other iliac artery. The second section of the device includes a tubular graft that can be advanced through the other iliac artery into engagement with the opening in the main body. This arrangement also is awkward to place and presents additional difficulties. Among those difficulties is that where the body and one of the legs is formed in a unitary structure, the device similarly does not lend itself to modular construction in which the individual components can be combined to match the dimensions of the particular patient's anatomy. Also among the difficulties with the device is that it employs stenting elements formed from a shape memory alloy that is not readily visualized under fluoroscopic examination and must be placed relatively quickly, before the stent expands as a consequence of exposure to body temperature.

WO 98/23242

PCT/US97/21211

- 3 -

A third approach, described in PCT application PCT/DK94/00468 (International Publication No. WO95/16406) employs an endovascular device for placement at the region of an arterial bifurcation that includes a three-component system including a main, bag-like body intended for placement in the aorta. The bag-like body has a pair of openings formed at its lower end. Each of the openings is said to receive an end of a tubular prosthesis inserted through each of the iliac arteries. The tubular prostheses are said to attach to the main bag-like body and extend into the iliac arteries. Among the apparent difficulties with this arrangement are that there is no way for the physician to visualize, fluoroscopically, the main bag-like body or the location of the openings that must be accessed in order to insert the leg segments into the openings. Additionally, the apparently flexible structure of the bag-like body would enable the bag to flex under the influence of blood flow, body movement and engagement with the apparatus for delivering and placing the leg segments, all of which would present considerable difficulties in the placement process. Moreover, even if the leg segments could be attached to the main body, the apparent relationship of the leg segments with the main body is such as to present an irregular, turbulent flow path from the main body to the leg extensions.

None of the prior art relating to the placement of a bifurcated tubular endoprosthetic implant within the region of the aortic-iliac arteries has suggested a modular construction by which the components can be accurately positioned, assembled and, if necessary, is recaptured within the delivery device so that the module can be redeployed in its proper position or removed in its entirety. Additionally, none embodies an arrangement in which the leg portions of the stent have a high degree of flexibility in order to conform easily to the configuration of the particular patient's vascular anatomy.

It would be desirable to provide a modular implant that can be constructed in situ with modules that can be accurately placed and connected easily with individual modules selected to conform closely to the vascular anatomy of the

individual patient. It is among the general objects of the invention to provide such a modular implant construction.

Summary of the Invention

The endoprosthetic implant of the present invention is formed from separate components that are individually and sequentially inserted

transluminally to the region to be treated such as, for example, the region of the abdominal aorta and iliac arteries. Each is deployed in sequence by a catheter-like delivery device. Except for the first placed module, each module is

connected to a previously placed module. The first placed module comprises a trunk adapted to be placed in the aorta and having a relatively large upstream opening and a pair of smaller downstream openings. Each of the downstream openings is adapted to receive the upstream end of one of two tubular leg

extensions. The trunk, which is constructed to be recapturable within the delivery device, includes a tubular synthetic graft having upstream and downstream ends and a resilient expandable frame assembly. The frame assembly includes a

radially expandable anchor at its upstream end that serves to secure the endoprosthesis to healthy aortic tissue and also maintains the upstream end of the endoprosthesis expanded and in sealed engagement with the lumen of the aorta. A stent at the downstream end of the graft maintains the downstream

branches of the graft open and receptive to the leg extensions. The anchor and the stent are connected to each other by at least two longitudinal struts in a manner that enables the trunk to be recaptured within the delivery device and repositioned or removed. The struts, anchor and stent also provide sufficient

longitudinal stiffness and column strength for the trunk so that it will not buckle when engaged by the leg extensions or the delivery device by which the leg

extensions are placed. The frame assembly is such that the trunk is relatively stiff to assure that it will remain securely in place to present a stable target that can be accessed by the other modular components with improved facility. The

leg extensions are constructed to facilitate their bending without kinking in order to conform to the specific anatomy of the patient. The modular construction of the endoprosthesis enables it to be formed from components, each of which can be selected to fit the specific part of the vascular anatomy of the patient into which it is to be placed.

It is among the general objects of the invention to provide an improved endoluminal implant adapted to be placed in a bifurcated vascular region. Another object of the invention is to provide an arrangement of modular endoluminal implant components by which an endoluminal graft may be constructed within the vascular lumen to a configuration conforming to the patient's vascular anatomy.

Another object of the invention is to provide an arrangement of modular endoluminal implant components including a trunk for placement within a blood vessel and legs connectible to the trunk for individual placement in a branch blood vessels. An additional object of the invention is to provide a modular graft of the type described in which each of the individual modules can be positioned accurately and in which at least the first placeable module can be recaptured and repositioned, if necessary. Another object of the invention is to provide an improved method for construction of an endoluminal implant in situ at a bifurcated region.

Description of the Drawings

The foregoing and other object and advantages of the invention will be appreciated more fully from the following further description thereof, with reference to the accompanying drawings, of which:

FIG. 1 is a diagrammatic illustration of a portion of an abdominal aorta illustrating, in phantom, an aortic aneurysm confined to the aorta;

FIG. 2 is an enlarged illustration similar to FIG. 1 but with an aneurysm that has involved a substantial length of the abdominal aorta and has extended into the iliac arteries, with an implant in accordance with the invention operatively positioned in the region of the aneurysm.

FIG. 3 is an illustration of the trunk module of the endoprosthetic implant; FIG. 4 is an illustration of an individual resilient component that may be used as an anchor or a stent;

FIG. 4A is an illustration of the region of connection between a strut and a straight segment of the stent;

FIG. 5 is an illustration of the juncture of the ends of the wire that forms the resilient component of FIG. 4;

FIG. 6 is an illustration of the frame assembly for the trunk component of the implant, including an anchor, a stent and a plurality of longitudinal struts extending between the anchor and stent;

FIG. 7 is a greatly enlarged longitudinal section of a portion of a strut of the trunk;

FIG. 8 is an illustration of an embodiment of a hook and hook support attached to a portion of the anchor as seen from a location radially outward of the anchor and viewed in a radially inward direction;

FIG. 9 is an illustration of the hook and hook support of FIG. 8 as seen from the left of FIG. 8 and as viewed in a direction generally tangential of the anchor;

FIG. 10 is an illustration of an anchor having the hook configuration illustrated in FIGS. 8 and 9 as withdrawn into a pod at the distal end of a delivery device;

FIG. 11 is an illustration similar to FIG. 8 of a detent carried by the anchor at the upper end of the trunk engagable with the tissue of a body lumen to prevent movement of the anchor in an upstream direction after the endoprosthesis has been deployed;

- FIG. 12 is an enlarged side elevation of the bent tip at the end of the detent of FIG. 11;
- FIG. 13 is a top view of the detent arrangement of FIG. 11;
- FIG. 14 is an illustration of the upstream end of a trunk embodying alternating hooks to resist downstream movement and detents to resist upstream movement of the endoprostheses;
- FIG. 15 is an illustration of an embodiment of a leg extension that may be used in the practice of the invention, shown in its low profile, unexpanded configuration;
- FIG. 16 is a fragmented illustration of the leg segment shown in FIG. 15 after being expanded; and
- FIG. 17 is an illustration of the manner in which the upstream end of a leg extension engages the trunk when the two are connected;
- FIG. 18 an illustration as seen along the line 18-18 of FIG. 17;
- FIG. 19 is an illustration of a modified embodiment of the trunk module of the invention;
- FIG. 20 is an end view of the lower end of the trunk as shown in FIG. 19 as seen from 20-20 of FIG. 19;
- FIG. 21 is a reduced scale, longitudinal cross-section through the trunk of FIG. 19 as seen from 21-21 of FIG. 19;
- FIG. 22 is a fragmented illustration of a deployment catheter having a modified arrangement for releasably gripping the trailing end of an endoprostheses module;
- FIG. 23 is a fragmented, sectional, diagrammatic illustration of the endoprostheses gripping arrangement of FIG. 22, enlarged, and illustrating the gripping members projected distally of the end of the delivery sheath;
- FIG. 24 is an illustration similar to FIG. 23 with the gripping mechanism having been operated to release the trailing end of the endoprostheses and with the endoprostheses as shown in an expanded configuration;

FIGS. 25A-25F illustrate, schematically, sequential steps in the placement of the endoprosthesis;

FIGS. 26D-26G illustrate, schematically, a modified procedure of sequential steps in the placement of the endoprosthesis; and

FIG. 27 is a diagrammatic illustration of the manner in which the modified trunk of FIG. 19 may be placed.

5

Description of the Preferred Embodiment

FIG. 1 illustrates, diagrammatically, the region of the human aorta 2 through which oxygenated blood is pumped from the heart in a downstream direction suggested at the arrows 4. Also shown are the renal arteries 6 that

10

branch off of the aorta to direct blood to the kidneys and the iliac arteries 8 that

branch at a bifurcation 10 to serve the lower extremities. FIG. 1 also illustrates

diagrammatically, and in phantom, an aneurysm 12 as may develop in the aorta 2 between the renal artery 6 and the bifurcation 10. The aneurysm 12 defines a

15

weakened region of the wall of the aorta and may be susceptible to rupture and

subsequent hemorrhaging under the influence of arterial blood pressure. Such a condition may be treated by placement of an implant within the artery to line and

reinforce the artery in the region of the aneurysm 12. The condition has been

treated, if at all, by attempting to place the implant surgically. Surgical placement presents a high risk to the patient. The present invention is directed to

20

placement of an implant assembly endoluminally by radially contracting the

implant within a sheath of a delivery catheter, inserting the catheter into a blood vessel to access the aneurysm, positioning the device within the aneurysm and

then releasing the implant assembly into engagement with supportive, healthy

25

arterial tissue beyond each end of the aneurysm.

In this description, a direction along which the delivery device is advanced (i.e., toward the heart) will be referred to variously as "leading", "forward", "above"

or "renal" and the opposite direction will be referred to variously as "trailing", "rearward", "below" or "iliac". Thus the tubular implants may be considered as having a leading end and a trailing end. When an implant has been advanced into and through the blood vessel from a downstream location to an upstream deployment location, the leading end of the implant also may be considered as being "upstream" and the trailing end as "downstream". For a device advanced in an upstream-to-downstream direction, the leading-trailing convention would be reversed.

It is not uncommon for the presence of an aneurysm to be undetected for a significant time, during which the extent of the aneurysm may increase. The aneurysm may develop both upstream and downstream along the abdominal aorta, extending into or beyond the bifurcation 10 into one or both of the iliac arteries 8. FIG. 2 represents such a condition in which the aneurysm has developed at its lower end to include involvement with both iliac arteries 8. When an aneurysm has developed to that stage, there no longer is sufficient healthy tissue to be securely engaged by a single tubular implant. Consequently, if the condition is to be treated by endoluminal placement of a prosthesis, the prosthesis will have to extend into one or both of the branch vessels.

FIG. 2 illustrates the assembled and deployed modules of an implant in accordance with the invention. The modules include a trunk, indicated generally at 14, and a pair of legs extensions, indicated generally at 16, 18. The trunk 14 is adapted to securely engage a region of healthy, supportive arterial tissue 20 above the aneurysm 12. When deployed, the lower end of the trunk 14 extends into the region of the aneurysm and is arranged to receive the upper ends of leg extensions 16 and 18 in a secure connection. The lower ends of the leg extensions 16, 18 are arranged to extend into and engage healthy tissue in the

iliac arteries. When the endoprosthetic implant is fully deployed, it will define flow channels for blood from healthy vessel tissue above the aneurysm to healthy vessel tissue below. Over time, and depending on the construction of the

implant, tissue can be expected to grow into the wall of the implant and ultimately approximate a natural biological luminal surface. The region 13 within the aneurysm exteriorly of the implant typically can be expected to be filled with mural thrombus.

Each of the trunk 14 and leg extensions 16, 18 is placed endoluminally and separately, with the trunk 14 being placed first. The components are

generally tubular and may be placed with a catheter-like delivery device,

indicated diagrammatically at 15 in FIG. 19B, as described in European patent application 95114543.2 published March 20, 1996 (Publication No. EP

701800A1), the disclosure of which is incorporated herein by reference, in its entirety. The delivery device 15 includes an elongate flexible tubular sheath 17

that defines a tubular pod 19 at its leading end. The pod 19 is adapted to contain an expandable tubular endoprosthesis, such as a trunk 14 or one of the leg

extensions 16, 18, in a radially contracted, low profile configuration. When the delivery device 15 has been advanced to the intended site of deployment, the

tubular endoprosthesis is maintained in position by a staying member (not shown) disposed within the sheath while the delivery sheath and pod are

withdrawn. As the sheath and pod withdraw, the leading end of the endoprosthesis is progressively exposed and progressively expands into

engagement with the blood vessel. The delivery device and trailing end of the endoprosthesis are configured so that they remain attached to the delivery

device 15 until the physician has had an opportunity to confirm that the endoprosthesis is in its desired position and orientation. The physician then can

complete withdrawal of the sheath and pod to completely release the implant in the patient. Alternately, if the implant is not in the desired position for orientation, the sheath can be readvanced forwardly to recapture the endoprosthesis for

repositioning or removal from the patient.

One embodiment of the trunk component 14 of the invention is illustrated in FIG. 3. The trunk 14 includes an elongate flexible tubular graft 22 that may be

of woven or other conventional vascular graft construction. The graft 22 of the trunk 14 preferably is bifurcated to include an upper single lumen portion 24 having a relatively large expanded diameter and a lower two-lumen portion 26 that includes bifurcated first and second branch tubes 28, 30. The techniques for constructing grafts having such a bifurcated structure are well known to those skilled in the art. Preferably the graft is of woven construction. Although the graft 22 includes the bifurcated branches 28, 30, the graft 22 is relatively short and is not intended itself to extend to the iliac arteries 8. Rather, the trunk 14 is constructed and selected so that the lower ends of the tubes 28, 30 will be disposed within the aneurysm, above the arterial bifurcation 10 and iliac arteries 8.

The trunk 14 should be formed to present a symmetrical internal configuration within its flow lumens, particularly in the bifurcated region 34. The bifurcate region 34 should define a relatively thin, smooth edge 35 (see FIGS. 17, 18) to the blood stream to minimize turbulence or regions of blood stagnation and to assure that the blood flow will be balanced and symmetrical in each of the legs 28, 30. Lack of symmetry or presentation of a broad region of bifurcation 34 could result in turbulent or asymmetrical blood flow that could lead to development of blood clots or other obstruction. The first and second tubular branches 28, 30 are attached to each other by one or more sutures 32 to maintain the tubes 28, 30 in close, generally parallel relation.

The trunk 14 includes a supporting frame, illustrated generally at 36 in FIG. 6. The frame 36 is connected to the graft 22 and serves to maintain the graft 22 in its open configuration as the trunk 14 is released within the artery. In the preferred embodiment, the frame 36 may include an anchor 38 at its upper end and a stent 40 at its lower end. The anchor 38 and stent 40 may be formed from a suitable wire such as MP35N alloy in a zigzag configuration as illustrated in FIG. 4, including a plurality of alternating straight sections 42 and bends 44. The anchor and stent may be formed by first bending the wire into the zigzag

configuration and then connecting the free ends 46 together, as by welding (FIG. 5) to define a ring-like configuration. Although omitted for clarity of illustration in FIG. 6, the anchor 38 may be provided with hooks, indicated generally at 48 as illustrated in FIGS. 1 and 3. The stent 40 is not intended to engage tissue and need not be provided with hooks 48 for that purpose. The lower ends of the stent 40 may protrude downwardly out of the legs 28, 30 and may serve as a connector to the delivery device.

By way of dimensional example, in the device intended for placement in an adult abdominal aorta, the overall length of the trunk 14 may be of the order of about six cm long, with the upper single lumen part 24 of the trunk being about three cm long and the lower portion 26 of the trunk also being about three cm long. The anchor 38 and stent 40 may be of the order 2.5 cm long so that when they are attached to the graft 22, the adjacently facing ends of the anchor 38 and stent 40 contained within the graft 22 will be spaced from each other to define an internal exposed cylindrical band 37 of uninterrupted graft material. The internal surface characteristics of the graft material preferably are such as to facilitate secure engagement with the leg extensions 16, 18 when the leg extensions are connected to the trunk 14, as described in further detail below. The large single lumen portion 24 of the trunk 14 may be of the order of fourteen to thirty mm in diameter. The diameter of the first and second tubular segments 28, 30 of the trunk may each be approximately half of that of the single lumen segment, that is, of the order of seven to fifteen mm. In a specific example, a trunk was made having a single lumen diameter of approximately 30 mm in diameter and a branch lumen diameter of approximately 14 mm. The anchor 38 is formed to define a relaxed diameter that is slightly greater than the diameter defined by the single tube portion 24 of the trunk to assure that the anchor will expand the open end of the graft fully. Similarly, the stent 40 is constructed to define a relaxed diameter that will assure full expansion of the branches 28, 30 and lower portion 26 of the endoprosthesis.

By way of dimensional example, in the device intended for placement in an adult abdominal aorta, the overall length of the trunk 14 may be of the order of about six cm long, with the upper single lumen part 24 of the trunk being about three cm long and the lower portion 26 of the trunk also being about three cm long. The anchor 38 and stent 40 may be of the order 2.5 cm long so that when they are attached to the graft 22, the adjacently facing ends of the anchor 38 and stent 40 contained within the graft 22 will be spaced from each other to define an internal exposed cylindrical band 37 of uninterrupted graft material. The internal surface characteristics of the graft material preferably are such as to facilitate secure engagement with the leg extensions 16, 18 when the leg extensions are connected to the trunk 14, as described in further detail below. The large single lumen portion 24 of the trunk 14 may be of the order of fourteen to thirty mm in diameter. The diameter of the first and second tubular segments 28, 30 of the trunk may each be approximately half of that of the single lumen segment, that is, of the order of seven to fifteen mm. In a specific example, a trunk was made having a single lumen diameter of approximately 30 mm in diameter and a branch lumen diameter of approximately 14 mm. The anchor 38 is formed to define a relaxed diameter that is slightly greater than the diameter defined by the single tube portion 24 of the trunk to assure that the anchor will expand the open end of the graft fully. Similarly, the stent 40 is constructed to define a relaxed diameter that will assure full expansion of the branches 28, 30 and lower portion 26 of the endoprosthesis.

The frame 36 also preferably includes a connection between the anchor 38 and stent 40 in the form of elongate struts 50. In the illustrative embodiment, one end of each of the struts 50 is attached to the stent 40, as by welding. The other end of each of the struts is connected to the anchor 38, as with sutures 52 that also secure the struts to the graft 22. The struts 50 which, preferably, are located exteriorly of the graft 22, also may be attached along their lengths to the exterior surface of the graft 22, as by heat bonding. The struts 50 should be connected to the anchor 38 and stent 40 in a manner that will reduce the risk of development of stress concentrations on the frame when the device is flexed at any time during its use. To that end, in the illustrative embodiment, the struts 50 may be attached, as described below, as by welding to the stent 40 and by sutures 52 that also serve to attach the anchor 38 and stent 40 to the graft 22. FIG. 7 shows, in greatly enlarged cross-sectional detail, the construction for the struts 50. The struts preferably include an inner core wire 54 surrounded by a helical coil 56 wrapped tightly about the core wire 54. The coil is wrapped in a thin tube of thermoplastic polymeric material 58. The polymeric layer may comprise polypropylene, applied as a tube about the coil 56 and then heated sufficiently to cause the polypropylene to begin to melt and flow into close intimacy with the turns of the coil 56 and the graft 22. The polymeric layer 58 may be formed from a lower melt temperature polymeric material from that of which the graft 22 is formed. By bonding the polymeric covering directly to the graft material, as suggested in FIG. 7, the struts may be attached securely along their full lengths to the graft 22 to provide full longitudinal support for the graft 22. The struts 50 also serve to prevent the graft 22 from becoming twisted in that the struts, being substantially straight and resilient, will resist such twisting. The core wire 54 and wire from which the coil 56 is formed may be formed from MP35N alloy. The construction of the struts provides enhanced longitudinal rigidity and column strength after the device is assembled and during deployment, while at the same time allowing the device to collapse to a low profile. A strut so

constructed may have sufficient radiopacity to permit adequate X-ray or fluoroscopic visualization of the struts when implanted in the abdominal aorta. The radiopacity of the struts may be enhanced by adding a radiopaque filler material to the polymeric material 58.

Although, in this embodiment, the lower, trailing end of the trunk 14 includes a pair of branch tubes 28, 30, a single stent 40 can be used to maintain both tubes 28, 30, in an open configuration when the device is deployed. The zigzag construction of the stent 40 is such that the adjacent portions 60 of the lower ends of the tubes 28, 30 can be placed between opposed pairs of straight sections 42 of the stent 40. FIG. 3 illustrates such an arrangement in which the adjacent straight sections 42a, 42b and opposed straight sections 42c, 42d embrace the adjacent portion 60 of the first and second tubes 28, 30. When the lower end of the trunk in this embodiment is relaxed and permitted to expand, the cooperation between the attached tubes 28, 30 and the stent 40 defines a generally oval cross-sectional configuration that includes the open adjacent tubes 28, 30. FIG. 6 illustrates the configuration of the frame with the stent 40 defining the generally oval shape. One or both of the tubes 28, 30 may be provided with radiopaque means for enhancing fluoroscopic visualization of the openings of the tubes 28, 30. Such means may, for example, be in the form of a ring of radiopaque material.

By way of further example, an anchor 38 adopted for use in an adult aorta may have twelve straight sections 42 disposed at an angle to each other of about 30°, when relaxed. It should be understood, however, that the dimensions and number of wire segments 42 of the anchor 38 may be varied, depending on the size of the lumen into which the endoprosthesis is to be placed and the specific condition to be treated. The diameter defined by the anchor should not be less than that of the body lumen into which it is to be deployed in order that the anchor may expand the graft fully into firm and sealed engagement with the body lumen. Preferably, the expanded diameter defined by the anchor may be slightly

greater than that of the body lumen. When the device is advanced to the site where it is to be implanted, it is released from the delivery device and, as it is released, the anchor expands to a larger diameter and into engagement with the inner surface of the body lumen. In the illustrative embodiment, the anchor 38 presses radially outwardly against the inner luminal surface of the aorta and serves to retain the trunk in place.

The security of the engagement between the trunk 14 and the blood vessel wall preferably is enhanced by providing hooks 48 on the upper anchor 38. The hooks 48 are formed on the upper ends of hook supports 47. The hook supports 47 preferably are formed from the same material as the wire of the anchor 38, and may be attached to and along the straight sections 42 of the anchor 38. The hook supports 47 and hooks 48 are arranged with the hooks 48 disposed above the bends 44 of the anchor 38. The hook supports 47 preferably are welded to the straight sections of the anchor at two junctions. The hooks 48 preferably are sharp and extend radially outward so that they can dig into the vessel to prevent migration of the device. The hooks 48 may be oriented at a downward angle to present substantial resistance to shifting of the upper anchor 38 in a downstream direction. The hooks 48 are arranged so that when the device is deployed, the hooks 48 will project radially outwardly beyond the outer portions of the endoprosthesis to assure that the hooks will engage securely the tissue of the blood vessel.

It is desirable that the device be constructed so that the anchor 38 can be contracted to a low profile configuration in which the implant is insertable into and carried by the tubular pod 19 of the delivery device 15 but without the hooks 48 becoming entangled with each other or otherwise interfering with the ability of the device to be radially contracted or expanded. To that end, the hooks are supported in a manner such that they will extend radially outwardly of the upper end of the delivery device when the implant is deployed but can be withdrawn radially inwardly into the pod of the delivery device when the implant is

contracted. FIGS. 3 and 8-10 illustrate a preferred arrangement by which the hooks may be provided with such radial movement. To that end the hook supports 47 are shaped to include an S-shaped region that defines transverse extensions E, F that can engage the rim 21 at the leading end of the pod 19 as the anchor 38 is drawn, relatively, into the pod 19. The S-shaped portion 62 of the hook support 47 may lie essentially in a single plane (see FIG. 9) that includes a center line 66 of the hook support 47 and extends approximately tangentially to the outer periphery of the anchor 38. The extent to which the transverse extensions E, F extend from the center line 66 may be varied depending on the other dimensional requirements of the system. The transverse extensions should define a distance E + F that will assure the retraction of the hooks 48 to their intended radially inwardly disposed configuration so that they can be captured within the pod 19, without entanglement, as suggested in Fig. 10. When the rim 21 of the pod 19 engages the transverse extensions E, F of the hook supports 47, advancement of the pod 19 will depress and urge the hook supports 47 radially inwardly to cause the ends of the hooks 48 to be drawn radially inwardly toward the central axis of the anchor. The chordal segment defined by the length E + F should be such that the radial projection J of the hook 48 will be well within the circumference defined by the inner diameter of the pod 19. Reference is made to European patent application, publication number EP701800A1, for additional description of the arrangements for effecting radial movement of hooks in response to engagement of the advancing pod.

It also may be desirable to include vessel-engaging members that will prevent shifting of the implant in an upstream direction. To that end and as shown in FIGS. 11-14 the anchor 38 also may be provided with detents 70 that may be formed on the upper ends of each of one or more detent supports 72 in the same manner as the hooks 48 are disposed on the hook supports 47. The detent supports 72 also may be provided with transverse extensions E' and F' to facilitate their controlled radial retraction when the pod 19 is advanced to

recapture the trunk. The detent 70 may be formed simply by providing a bent tip 74, at the upwardly extending ends of the supports 72, beyond the transverse

extensions. The bent tip 74 preferably is formed at an acute angle to the center line 76 of the support 72. By way of dimensional example, the bent tip 74 may be of the order of about 0.08" long and may extend radially outwardly by a

dimension K about 0.04 inch from the center line 76. The uppermost end of the tip may be beveled, as indicated at 78, to provide a sharp point oriented to dig into the tissue of the blood vessel should the device tend to shift in an upward direction. It should be noted that when the device is deployed the detents will

press radially outwardly against the tissue of the vessel. The sharp tips will not fully dig into the tissue of the vessel unless and until the device is urged in an upstream direction. The anchor 38 may be configured to have alternately

downstream resistant hooks 48 and upstream resistant detents 70 as shown in FIG. 14.

The stent 40 may be assembled and integrated with the graft 22 by first

attaching the lower ends of the inner core wires 54 to straight sections 42 of the stent 40, preferably in a manner that will avoid the development of significant

stress concentrations at the region of attachment. In the illustrative embodiment, the lower ends of the inner core wires 54 may be spot welded, as suggested at 53 in FIG. 4A. After the lower ends of the core wires 54 have been so attached,

the stent 40 is placed

in the open ends of the branch tubes 28, 30, passing the free ends of the inner core wires 54 from the inside to the outside of the graft 22 through small holes 51 formed in the branch tubes 28, 30. With the stent 40 positioned in the graft 22 as described with the core wires 54 protruding outwardly through the graft 22, the

helical coils 56 are slipped onto the core wires 54 and the polymeric tubes 58 are slipped over the helical coils 56. After the anchor 38 is assembled with its

arrangement of hooks 48 and, if employed, detents 70, the anchor 38 is placed

within the upper end of the graft 22, with the hooks 48, hook supports 47, detent

70 and detent support 72 being manipulated through small openings 53 formed about the upper end of the graft 22. The sutures are placed to further connect the anchor 38, stent 40, struts 52 and graft 22 together. The polymeric tubes 58 then may be heat bonded to the graft 22. It may be noted that the upper ends of the struts 50 need not be rigidly attached to the anchor 38 and, preferably, are attached to permit flexibility between the two without developing adverse stress concentrations. To that end, the sutures 52 associated with the anchor 38 provide a connection between the anchor 38 and the struts 50 while also serving to attach the anchor 38 to the graft 22. The sutures 52 associated with the anchor 40 serve to provide an additional connection between the frame 36 and the graft 22.

FIGS. 19-21 illustrate a modified embodiment of the anchor that may be constructed in similar fashion to that described above in connection with the embodiment of FIG. 3. In this embodiment, the graft 22' is formed to include an additional single lumen segment 27 having an expanded diameter approximately equal to the sum of the diameters of the first and second branch tubes 28', 30'. The stent 40 may be the same stent as that described above in connection with the embodiment of FIG. 3. The single lumen configuration of the segment 27 enables the stent 40 to expand that segment to a generally circular cross-section (FIG. 20). The struts 50' may be constructed in the same manner discussed above. The device thus may be considered to include a pair of generally circular cross-section lumens at its ends that communicate with a pair of smaller diameter parallel lumens defined by the tubes 28', 30'. As described below in connection with the description of the manner in which the device is used, the enlarged diameter opening defined by the segment 27 presents a larger target to facilitate coupling of the leg extension 16', 18, with the trunk.

As shown in FIGS. 15-18, each of the leg extensions 16, 18 may include a flexible outer tube 90 of the type commonly used as a synthetic blood vessel. Although other constructions may be employed, in a presently preferred

embodiment the tube 90 may be formed from a conventional graft material, such as a fabric similar to the fabric from which the graft 22 is formed. It should be understood, however, that any of a variety of conventional graft materials may be employed including graft materials that have differing characteristics than other of the modular components in order to suit the particular requirements of the patient. The length of the graft 90 may be varied to suit the anatomy of the particular lumens into which the implant is to be placed. The tube 90 is supported internally by a stent 92 that, in the preferred embodiment, extends substantially the full length of the tube 90. The lower end of the extension leg 16, 18 may be provided with a means by which it can be engaged by the delivery catheter to enable the leg extension to be recaptured, for repositioning or removal before release, should that be desired. To that end lower end of the stent 92 may protrude downwardly beyond the lower end 91 of the tube 90 and preferably defines, when relaxed, a slightly flared configuration defining a plurality of downwardly facing projections 94. Stent 92 is expandable from a low profile configuration (FIG. 15) in which it can be received within the tubular pod 19 of the delivery device and an expanded configuration in which it has fully expanded the graft 90. Although a number of stents may be employed, it is presently preferred to use the type of stent described in German patent number 43 03 181.1 issued to Angiomed AG of Karlsruhe, Germany and from whom such stents are available commercially.

The leg extensions 16, 18 are deployed with the use of a delivery catheter such as that described above in connection with the trunk 94 and incorporated by reference herein. One of the leg extensions 16, 18 is carried by the delivery device to a position in which the leg extension is disposed within one of the branch tubes 28, 30 of the previously placed trunk 14. While maintaining the position of the leg extension, the sheath and pod 19 are withdrawn to progressively enable the stent 92 to expand the tube 90 within and into engagement with the inner surface of the trunk 14. The leg extensions 16, 18

are selected to have an expanded diameter to match the internal dimensions of

the trunk 14 so that the upper end of the leg extension, when released, will firmly and securely engage the inner luminal surfaces of the trunk 14. The dimensions and engagement should be such as to assure a firm and secure contact between

the inserted end of the leg extensions to prevent separation of the leg extension from the trunk 14 as well as to provide a seal between the two to prevent blood from leaking out of the implant. The preferred embodiment the leg extensions are secured by cooperative engagement of the facing surfaces of the tube 90 and the inner surface of the graft 22 coupled with the radial expansive force with which the stent 92 presses the tube 90 against the interior of the truck 14.

Preferably a substantially region of surface-to-surface engagement will result between the coextensive circumferential band 37 of graft material 22 of the trunk

14 with the external engaged surface of the upper end of the tubular graft 90. Depending on the configuration at the lower end of one or more of the

modules, it may be desirable to provide a delivery device modified somewhat from that described in European published application No. EP 0 701 800 A1, particularly with the manner in which the lower (trailing) end of the module is held. As shown in FIGS. 22-24, the modified delivery device includes an

arrangement of an outer flexible tube 96 that defines a slightly enlarged diameter sheath 98 at its distal end. Disposed coaxially within the outer tube 96 is an

intermediate tube 100 that is slidably longitudinally within the outer tube 98 and has a distally opening cup 102 at its distal end. A metal inner tube 104 is disposed coaxially within the intermediate tube 100 for longitudinal movement with respect to the intermediate tube 100. The inner tube has an enlarged

member 106 attached at a location that the member 106 can be disposed within the cup 102 (FIG. 23) or extended distally beyond and out of the cup 102 (FIG. 24). The cross-sectional dimensions of the member 106 and the inner surface of

the cup 102 are such that when brought together they can cooperate to wedge the trailing end of a radially contracted endovascular modular component such as

a leg extension 16, 18 between the member 106 and the cup. As illustrated diagrammatically in FIG. 23, the trailing end of the leg extension 16 is securely gripped in the generally annular space between the member 106 and the cup 102. The grip should be secure to assure that the trailing end of the endoprosthesis will not be released inadvertently so that the endoprosthesis can be recaptured, should that be desired. FIG. 23 illustrates the relative configuration of the components after the outer tube 96 has been withdrawn sufficiently to withdraw the sheath 98 to project the gripped, trailing end of the endoprosthesis 16 out of the sheath. When the physician is satisfied that the endoprosthesis 16 has been placed as desired, the intermediate and inner tubes 100, 104 can be moved relative to each other to release the endoprosthesis 16 so that the endoprosthesis can expand (FIG. 24).

The position of the tubes 96, 100, 104 may be controlled by conventional lockable fittings at the proximal end of the device. As shown in FIG. 22 a fitting 108 is attached to the proximal end of the tubular shaft 96. The intermediate tube 100 extends through the fitting 108 and itself has a fitting 110 at its proximal end. The inner tube 104 extends through the fitting 110 and has another fitting 112 attached to its proximal end. The fitting 112 is constructed to enable a guidewire (not shown) to be inserted through the lumen of the inner tube 104. FIGS. 25A-25F illustrate, diagrammatically one sequence of the operations by which the modular endoprosthesis may be deployed. FIG. 25A illustrates, diagrammatically, a portion of a patient's abdominal aorta 2 and several branch vessels, including the renal arteries 6 and iliac arteries 8. The aneurysm 12 is illustrated as having extended into and beyond the bifurcation 10, to include a portion of the iliac arteries 8. FIG. 25A illustrates an access opening 82 formed in one of the iliac arteries 8. The access opening 82 may be formed percutaneously or in a surgical cut-down technique. Typically, an introducer sheath (not shown) will be placed through the opening 82 to receive the various instruments and permit their manipulation without subjecting the patient to

excessive trauma. FIG. 25A illustrates the patient anatomy with a guidewire 84 having been placed to extend upwardly to and through a region of healthy aortic tissue 3 above the aneurysm 12. With the guidewire 84 in place, the delivery device, which includes a guidewire lumen, is advanced over the guidewire 84 until the pod 19 at the distal end of the sheath 17, which contains the trunk 14 in a low profile, contracted configuration, is located at the intended placement site. When the physician is satisfied that the pod 19 and trunk 14 are at the desired location (FIG. 25B), the delivery catheter 15 is manipulated to maintain the position of the trunk 14 relative to the patient's vasculature, while withdrawing the sheath 17 and pod 19, as indicated by the arrow 85 in FIG. 25C. The desired position of the trunk 14, before deployment, is such that the anchor 38, including its hooks 48 and detents 70, will be disposed within healthy tissue capable of firmly supporting the upper end of the trunk 14. As suggested in FIG. 25C, as the sheath 19 is withdrawn, the trunk 14 is progressively exposed to enable the anchor 38 to expand and the endoprosthesis toward an expanded diameter so that it will firmly and securely engage the region 3 of healthy aortic tissue above the aneurysm 12.

Should it be necessary reposition or withdraw the trunk 14, even after its anchor 38 has engaged the healthy tissue 3, that can be accomplished at any time before complete release by simply readvancing the sheath and pod 19 upwardly over the trunk 14. As the rim of the sheath 19 engages the transverse extensions, the hooks 48 and detents 70 are retracted radially inwardly within the circumference of the rim of the pod 19 so that further advancement of the pod will fully enclose the hooks 48 and detents 70 in the manner suggested in FIG. 10. After the physician is satisfied that the device is in the desired positioned and orientation, the delivery catheter is manipulated to release the trailing end of the trunk 14.

FIG. 26D illustrates the configuration of the trunk 14 after it has been released. In this configuration the trunk 14 is attached to the healthy aortic tissue

only by the anchor 34. The lower end of the trunk 14, including the lower ends of the bifurcated tubes 28, 30 depend downwardly but without support of engagement with any part of the body lumen. The construction of the trunk is such that it has sufficient longitudinal stiffness and the open lower ends are supported by the stent 40 so that it has sufficient rigidity to be self supporting and readiness to receive leg extensions 16, 18. After the trunk 14 has been deployed, the delivery device is removed from the patient. In one method of deployment, the guidewire 84 may remain in place in order to serve as a guide for delivery device for one of the leg extensions 16, 18.

From foregoing it will be appreciated the trunk 14 serves as a first, securely placed component of the endovascular prosthesis. The trunk 14 is configured to present a stable pair of targets in the form the open lower ends of the branch tubes 28, 30 in order to facilitate advancement of the leg extensions into the branch tubes 28, 30. The frame associated with the trunk 14 provides a firm stable shape for the trunk 14 that will be unaffected by engagement of the delivery device for the leg extensions. The trunk 14 provides continuous wide inlet openings to receive the upper, leading ends of the leg extensions 16, 18. The lower openings of the branch tubes 28, 30 may be provided with radiopaque markers, as in the form of rings 29 or the like by which the entry openings of the branch tubes 26, 28 can be visualized fluoroscopically.

The placement of the leg extensions 16, 18 may be performed in essentially the same manner as the placement of the trunk 14, that is, by a catheter-like delivery device adapted to contain a leg extension in a low profile configuration, in readiness for expansion when released. After the trunk 14 as been placed, a delivery device is loaded with one of the leg extensions 16, 18. The delivery device then can be advanced over the initially placed guidewire 84 until its leading, upper end is disposed, as desired, within the trunk 14. As shown in FIGS. 17 and 18 the leg extension may be advanced into a receptive of the branch tubes 28, 30 to dispose the upper end of the inserted leg extension

beyond the stent 40 and into the intermediate 37 between the stent and anchor. As described, the surface characteristics of the outside of the tube 90 and the interior of the trunk, including the internal surfaces of the graft material 22 should be selected so that a secure and sealed connection will be formed when the tube 90 is in its expanded configuration, connected to the trunk 14. When the leg extension is so placed, the sheath and pod of the delivery device 15 are withdrawn to enable the leg extension to expand and with its upper portion and secure overlapped engagement with the trunk 14. As the sheath and pod are progressively withdrawn the exposed portion of the stent can expand to its expanded diameter. The length and diameters of the leg extension are selected so that the upper end will securely engage the trunk and the lower end will expand into firm engagement with healthy tissue of the iliac artery 8, below the aneurysm 12. Presently preferred embodiment, the lower of the leg extensions include the downwardly and radially outwardly extended projections adapted to engage healthy tissue of the iliac arteries. When the delivery device has been withdrawn, the projections will remain in engagement with healthy iliac artery tissue.

The in vivo construction of the bifurcated graft then can be completed by placing another guide wire 86 in the other iliac artery and advancing it upwardly through the other of the bifurcated tubes 28, 30. The delivery device, loaded with the other leg extension than can be advanced in the same manner as the first leg extension and deployed in the same manner. FIG. 26E illustrates the withdrawal of the delivery device as the other leg extension expands progressively. FIG. 26F illustrates the bifurcated endoprosthesis, constructed in modular fashion after removal of the guide wires and delivery devices.

FIGS. 26D-26F illustrate a modified procedure for placing the modular endoprosthesis. The modified procedure begins the same as that described above in connection with FIGS. 26A-26C. The next step, of delivering and deploying one of the leg extensions 16, 18, is substantially similar in this modified

procedure except that instead of directing the guidewire and delivery device into the bifurcated branch of the trunk on the same side as the iliac artery that was accessed, the delivery device is directed to the branch tube 30 on the opposite side. By so doing, the placement of the initial guidewire and the delivery device is facilitated in that the branch tube 30 on the opposite side can be expected to be more directly in line with the iliac artery through which the device was placed. FIG. 26D illustrates the first of the two leg extensions having been so cross-

placed. FIG. 26E illustrates the system after the leg extension has been attached to the trunk and the delivery device has been withdrawn, leaving one of the leg extensions in place connecting the trunk and its associated iliac artery.

FIG. 26F illustrates the similar placement of the other leg extension, showing the delivery device having partially deployed the leg extension in the other of the branch tubes. FIG. 26F illustrates that the cross-placement results in the devices

being crossed within the aneurysmal region. FIG. 26G illustrates the

configuration after the second of the leg extensions has been fully deployed to directly connect its associated branch tube of the trunk with its associated iliac

artery. It should be understood that variations of this modified procedure may be employed. For example, it may be desirable to first deploy both guidewires G1,

G2 in a cross-configuration. Then, with the guidewires in place, the delivery

devices may be advanced over the guidewires and the module deployed.

FIG. 27 illustrates, diagrammatically, the manner in which the modified

trunk shown in FIG. 19 may be used in the practice of the invention. The

placement and deployment of the trunk itself as well as the leg extensions is

essentially identical to the modes described above. The addition of the lower

segment 27, however, provides a larger tubular target for the guidewires,

illustrated diagrammatically as G1 and G2. The physician may find it easier to

place the guidewire within the larger diameter lower extension than if the target

were the smaller diameters as defined by the branch tubes 28, 30. The distal

ends of the guidewires typically will be provided with an atraumatic J-shape. Use

of the cross-over technique described above in connection with FIGS. 27D-27G may be employed, as shown.

It should be understood that the foregoing description of the invention is intended merely to be illustrative thereof and other embodiments, modifications and equivalents will be apparent to those skilled in the art without the departing from the principles of the invention.

Having thus described the invention what we desire to claim and secure by letters patent is:

5

- 1 1 A modular, endoluminally placeable endoprosthetic implant for placement in a bifurcated region of a body lumen comprising:
- 3 a longitudinally stiff, tubular trunk having an upper segment defining a main single tube having an open upper end and adjacent segment defining a pair of tubular branches communicating with the single tube and having open lower ends;
- 7 the trunk being radially collapsible to a low profile and expandable from the low profile to an expanded diameter;
- 9 an anchor disposed at the open end of the single tube segment of the trunk; and
- 11 a pair of tubular leg extensions each having upper and lower ends, each upper end being contractible radially to a low profile to enable it to be inserted into the open lower end of one of the tubular branches of the trunk, each leg extension being expandable to a configuration in which its upper end is engageable with the interior of the trunk to effect attachment of the leg to the trunk and to define a continuous lumen from the upper portion of the trunk to and through the leg extensions.
- 1 2. An implant as defined in claim 1 wherein the trunk comprises a flexible tubular graft and an anchor connected to the upper portion of the graft to support the graft in an expanded configuration and to engage the body lumen.
- 1 3. An implant as defined in claim 2 wherein the graft of the trunk is bifurcated to include the main tube and the branch tubes, the branch tubes being connected and supported in substantially parallel relation to each other and to the main tube.
- 4

Claims

1 4. An implant as defined in claim 2 wherein the graft is bifurcated to
2 define the branch tubes, the implant having a stent engageable with the ends of
3 the branch tubes to maintain the branch tubes in an expanded, side by side
4 configuration that, in transverse cross section, defines generally an oval that
5 includes the two branch tubes.

1 5. An implant as defined in claim 1 wherein the graft is bifurcated to
2 define the branch tubes, the implant having a stent engageable with the ends of
3 the branch tubes to maintain the branch tubes in at expanded, side by side
4 configuration that, in transverse cross section, defines generally an oval that
5 includes the two branch tubes.

1 6. An implant as defined in either one of claims 4 or 5 wherein:
2 the upper ends of the leg extensions are constructed to be securely
3 engageable with the internally exposed surface of the graft.

1 7. An implant as defined in any one of claims 1 to 6 further
2 comprising:
3 a radiopaque element disposed in association with the branch
4 tubes to enable radiographic visualization of the location of the open ends of the
5 branch tubes.

1 8. An implant as defined in claim 7 wherein the radiopaque element
2 comprises a ring-defining radiopaque member disposed about the open end of at
3 least one of the branch tubes.

1 9. An implant as defined in claim 1 wherein the implant is stiffened
2 longitudinally by longitudinally extending struts.

- 1 16. An implant as defined in claim 15 wherein the radially protruding members include at least one downwardly extending hook and at least one upwardly protruding member having a radially outwardly bent tip.
- 2 15. An implant as defined in claim 1 further comprising:
 1 including at least one protrusion engageable with the body lumen to prevent movement of the trunk in an upward direction and at least one protruding member engageable with the body lumen to prevent movement of the trunk in a downward direction.
- 2 14. An implant as defined in claim 1 wherein the stent has a connector at its lower end for releasable attachment to a delivery device.
- 1 13. An implant as defined in claim 9 wherein the struts have sufficient longitudinal stiffness to transmit a portion of a radially inward contracting force applied at the stent to the anchor, and for that force to increase as it is applied progressively along the struts in a direction toward the anchor.
- 2 12. An implant as defined in claim 11 further comprising the struts being attached to the anchor and the stent.
- 1 11. An implant as defined in claim 11 wherein the struts extend along the main tube and branch portions of the trunk.
- 2 10. An implant as defined in claim 9 wherein the struts are disposed externally of and are attached to the graft.

17. An implant as defined in claim 16 wherein each hook and each bent tip is mounted on the end of a flexible support, the support being attached to the anchor for radially inward and outward movement.

18. An implant as defined in claim 1 further comprising:
the tubular trunk having a lower segment adjacent and defining a continuation of the tubular branches, the lower segment having a single lumen and a diameter that is greater than the diameter of either of the tubular branches.

19. An implant as defined in claim 18 wherein the diameter of the lower tubular segment is approximately equal to the sum of the diameters of the tubular branches.

20. An implant as defined in claim 18 further comprising:
a radiopaque element disposed in association with the lower single lumen segment to enable radiographic visualization of the location of the lower single lumen segment.

21. An implant as defined in claim 20 wherein the radiopaque element comprises a ring-defining radiopaque member disposed about the open end of the lower single lumen segment.

22. An implant as defined in claim 18 further comprising:
a stent engageable with the single lumen lower segment to maintain the lower segment in an expanded configuration.

23. An implant as defined in claim 22 wherein the expanded configuration is substantially circular.

- 4 single tube having an open upper end and a lower segment defining a pair of
- 3 a flexible bifurcated graft having an upper segment defining a main
- 2 placement in a bifurcated region of a body lumen comprising:
- 1 26. A modular, endoluminally placeable endoprosthetic implant for
- 23 extensions into the tubular branches may be facilitated.
- 22 ends of the tubular branches in a stable position where insertion of the leg
- 21 the means for stiffening the trunk being sufficient to maintain the open
- 20 from the upper portion to the trunk to and through the leg extension;
- 19 attachment of the leg extension to the trunk and to define a continuous lumen
- 18 the leg extension is engageable with the interior of the trunk to effect the
- 17 the trunk and being expandable to a configuration in which the upper portion of
- 16 profile to enable it to be inserted into the open end of one of the branch tubes of
- 15 upper end of each of the leg extensions being contractable radially to a low
- 14 pair of tubular leg extensions having upper and lower ends, the
- 13 means for imparting longitudinal stiffness to the trunk;
- 12 the trunk;
- 11 an anchor disposed at the open end of the single tube segment of
- 10 from the low profile to an expanded diameter;
- 9 the trunk being radially collapsible to low profile and a expandable
- 8 branches in communication with the single tube and having open lower ends;
- 7 tube having an open upper end and a lower segment defining a pair of tubular
- 6 a tubular trunk having an upper segment defining a main single
- 5 replacement in a bifurcated region of a body lumen comprising:
- 4 25. A modular, endoluminally placeable endoprosthetic implant
- 3
- 2 at its lower end for releasable attachment to a delivery device.
- 1 24. An implant as defined in claim 20 wherein the stent has a connector

5	tubular branches in communication with the single tube, the tubular branches having open lower ends;	6
7	frame means for supporting the graft to impart longitudinal stiffness to the graft while enabling the graft to be collapsed radially to a low profile and to enable expansion of the graft from a low profile to an expanded cross-sectional configuration.	10
1	27. An implant as defined in either of claims 25 or 26 further comprising means at the upper end of the implant for engaging healthy tissue defining the body lumen and for precluding movement of the implant in at least one of upward or downward directions within the body lumen.	4
1	28. An implant as defined in either one of claim 1 or claim 18 wherein at least one of the leg extensions comprises a tubular member and a stent extending the full length of the tubular member, the stent having an expanded diameter that is no less than the diameter of the expanded tubular member, the expanded tube having a diameter that is no less than that of at least one of the branch tubes of the trunk.	1
2	29. An implant as defined in claim 28 wherein at least one of the leg stents has a connector at its lower end for connection to a delivery device.	2
1	30. An implant as defined in claim 28 wherein the stent is bendable without kinking.	2
1	31. An implant as defined in claim 28 wherein the upper end of the stent does not extend upwardly beyond the end of the branch tube.	2

- 1 35. An endoluminally placeable endoprosthetic implant for placement in
2 the abdominal aorta comprising:
3 a tubular trunk having an upper segment defining a main single
4 tube having an open upper end and a lower segment defining a pair of tubular
5 branches in communication with the single tube, the tubular branches having
6 open lower ends;
7 the trunk being radially collapsible to a low profile and expandable
8 from the low profile to an expanded diameter;
9 an anchor disposed at the upper end of the single tubes segment
10 engageable with healthy aortic tissue disposed upwardly of an abdominal
11 aneurysm;
12 the lower end of the trunk being adapted to depend freely within the
13 aneurysm;
14 the trunk including a frame constructed to impart longitudinal
15 stiffness to the trunk and to maintain the lower ends of the branch tubes open.
- 1 34. An implant as defined in claim 28 wherein the lower ends of the
2 stent have radially outwardly projecting members arranged to define a greater
3 diameter than that of the expanded tube, the radially outwardly projecting
4 members being engageable with a body lumen to prevent downstream migration
5 of the leg extension.
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60
61
62
63
64
65
66
67
68
69
70
71
72
73
74
75
76
77
78
79
80
81
82
83
84
85
86
87
88
89
90
91
92
93
94
95
96
97
98
99
100
101
102
103
104
105
106
107
108
109
110
111
112
113
114
115
116
117
118
119
120
121
122
123
124
125
126
127
128
129
130
131
132
133
134
135
136
137
138
139
140
141
142
143
144
145
146
147
148
149
150
151
152
153
154
155
156
157
158
159
160
161
162
163
164
165
166
167
168
169
170
171
172
173
174
175
176
177
178
179
180
181
182
183
184
185
186
187
188
189
190
191
192
193
194
195
196
197
198
199
200
201
202
203
204
205
206
207
208
209
210
211
212
213
214
215
216
217
218
219
220
221
222
223
224
225
226
227
228
229
230
231
232
233
234
235
236
237
238
239
240
241
242
243
244
245
246
247
248
249
250
251
252
253
254
255
256
257
258
259
260
261
262
263
264
265
266
267
268
269
270
271
272
273
274
275
276
277
278
279
280
281
282
283
284
285
286
287
288
289
290
291
292
293
294
295
296
297
298
299
300
301
302
303
304
305
306
307
308
309
310
311
312
313
314
315
316
317
318
319
320
321
322
323
324
325
326
327
328
329
330
331
332
333
334
335
336
337
338
339
340
341
342
343
344
345
346
347
348
349
350
351
352
353
354
355
356
357
358
359
360
361
362
363
364
365
366
367
368
369
370
371
372
373
374
375
376
377
378
379
380
381
382
383
384
385
386
387
388
389
390
391
392
393
394
395
396
397
398
399
400
401
402
403
404
405
406
407
408
409
410
411
412
413
414
415
416
417
418
419
420
421
422
423
424
425
426
427
428
429
430
431
432
433
434
435
436
437
438
439
440
441
442
443
444
445
446
447
448
449
450
451
452
453
454
455
456
457
458
459
460
461
462
463
464
465
466
467
468
469
470
471
472
473
474
475
476
477
478
479
480
481
482
483
484
485
486
487
488
489
490
491
492
493
494
495
496
497
498
499
500
501
502
503
504
505
506
507
508
509
510
511
512
513
514
515
516
517
518
519
520
521
522
523
524
525
526
527
528
529
530
531
532
533
534
535
536
537
538
539
540
541
542
543
544
545
546
547
548
549
550
551
552
553
554
555
556
557
558
559
560
561
562
563
564
565
566
567
568
569
570
571
572
573
574
575
576
577
578
579
580
581
582
583
584
585
586
587
588
589
590
591
592
593
594
595
596
597
598
599
600
601
602
603
604
605
606
607
608
609
610
611
612
613
614
615
616
617
618
619
620
621
622
623
624
625
626
627
628
629
630
631
632
633
634
635
636
637
638
639
640
641
642
643
644
645
646
647
648
649
650
651
652
653
654
655
656
657
658
659
660
661
662
663
664
665
666
667
668
669
670
671
672
673
674
675
676
677
678
679
680
681
682
683
684
685
686
687
688
689
690
691
692
693
694
695
696
697
698
699
700
701
702
703
704
705
706
707
708
709
710
711
712
713
714
715
716
717
718
719
720
721
722
723
724
725
726
727
728
729
730
731
732
733
734
735
736
737
738
739
740
741
742
743
744
745
746
747
748
749
750
751
752
753
754
755
756
757
758
759
760
761
762
763
764
765
766
767
768
769
770
771
772
773
774
775
776
777
778
779
780
781
782
783
784
785
786
787
788
789
790
791
792
793
794
795
796
797
798
799
800
801
802
803
804
805
806
807
808
809
810
811
812
813
814
815
816
817
818
819
820
821
822
823
824
825
826
827
828
829
830
831
832
833
834
835
836
837
838
839
840
841
842
843
844
845
846
847
848
849
850
851
852
853
854
855
856
857
858
859
860
861
862
863
864
865
866
867
868
869
870
871
872
873
874
875
876
877
878
879
880
881
882
883
884
885
886
887
888
889
890
891
892
893
894
895
896
897
898
899
900
901
902
903
904
905
906
907
908
909
910
911
912
913
914
915
916
917
918
919
920
921
922
923
924
925
926
927
928
929
930
931
932
933
934
935
936
937
938
939
940
941
942
943
944
945
946
947
948
949
950
951
952
953
954
955
956
957
958
959
960
961
962
963
964
965
966
967
968
969
970
971
972
973
974
975
976
977
978
979
980
981
982
983
984
985
986
987
988
989
990
991
992
993
994
995
996
997
998
999
1000
1001
1002
1003
1004
1005
1006
1007
1008
1009
1010
1011
1012
1013
1014
1015
1016
1017
1018
1019
1020
1021
1022
1023
1024
1025
1026
1027
1028
1029
1030
1031
1032
1033
1034
1035
1036
1037
1038
1039
1040
1041
1042
1043
1044
1045
1046
1047
1048
1049
1050
1051
1052
1053
1054
1055
1056
1057
1058
1059
1060
1061
1062
1063
1064
1065
1066
1067
1068
1069
1070
1071
1072
1073
1074
1075
1076
1077
1078
1079
1080
1081
1082
1083
1084
1085
1086
1087
1088
1089
1090
1091
1092
1093
1094
1095
1096
1097
1098
1099
1100
1101
1102
1103
1104
1105
1106
1107
1108
1109
1110
1111
1112
1113
1114
1115
1116
1117
1118
1119
1120
1121
1122
1123
1124
1125
1126
1127
1128
1129
1130
1131
1132
1133
1134
1135
1136
1137
1138
1139
1140
1141
1142
1143
1144
1145
1146
1147
1148
1149
1150
1151
1152
1153
1154
1155
1156
1157
1158
1159
1160
1161
1162
1163
1164
1165
1166
1167
1168
1169
1170
1171
1172
1173
1174
1175
1176
1177
1178
1179
1180
1181
1182
1183
1184
1185
1186
1187
1188
1189
1190
1191
1192
1193
1194
1195
1196
1197
1198
1199
1200
1201
1202
1203
1204
1205
1206
1207
1208
1209
1210
1211
1212
1213
1214
1215
1216
1217
1218
1219
1220
1221
1222
1223
1224
1225
1226
1227
1228
1229
1230
1231
1232
1233
1234
1235
1236
1237
1238
1239
1240
1241
1242
1243
1244
1245
1246
1247
1248
1249
1250
1251
1252
1253
1254
1255
1256
1257
1258
1259
1260
1261
1262
1263
1264
1265
1266
1267
1268
1269
1270
1271
1272
1273
1274
1275
1276
1277
1278
1279
1280
1281
1282
1283
1284
1285
1286
1287
1288
1289
1290
1291
1292
1293
1294
1295
1296
1297
1298
1299
1300
1301
1302
1303
1304
1305
1306
1307
1308
1309
1310
1311
1312
1313
1314
1315
1316
1317
1318
1319
1320
1321
1322
1323
1324
1325
1326
1327
1328
1329
1330
1331
1332
1333
1334
1335
1336
1337
1338
1339
1340
1341
1342
1343
1344
1345
1346
1347
1348
1349
1350
1351
1352
1353
1354
1355
1356
1357
1358
1359
1360
1361
1362
1363
1364
1365
1366
1367
1368
1369
1370
1371
1372
1373
1374
1375
1376
1377
1378
1379
1380
1381
1382
1383
1384
1385
1386
1387
1388
1389
1390
1391
1392
1393
1394
1395
1396
1397
1398
1399
1400
1401
1402
1403
1404
1405
1406
1407
1408
1409
1410
1411
1412
1413
1414
1415
1416
1417
1418
1419
1420
1421
1422
1423
1424
1425
1426
1427
1428
1429
1430
1431
1432
1433
1434
1435
1436
1437
1438
1439
1440
1441
1442
1443
1444
1445
1446
1447
1448
1449
1450
1451
1452
1453
1454
1455
1456
1457
1458
1459
1460
1461
1462
1463
1464
1465
1466
1467
1468
1469
1470
1471
1472
1473
1474
1475
1476
1477
1478
1479
1480
1481
1482
1483
1484
1485
1486
1487
1488
1489
1490
1491
1492
1493
1494
1495
1496
1497
1498
1499
1500
1501
1502
1503
1504
1505
1506
1507
1508
1509
1510
1511
1512
1513
1514
1515
1516
1517
1518
1519
1520
1521
1522
1523
1524
1525
1526
1527
1528
1529
1530
1531
1532
1533
1534
1535
1536
1537
1538
1539
1540
1541
1542
1543
1544
1545
1546
1547
1548
1549
1550
1551
1552
1553
1554
1555
1556
1557
1558
1559
1560
1561
1562
1563
1564
1565
1566
1567
1568
1569
1570
1571
1572
1573
1574
1575
1576
1577
1578
1579
1580
1581
1582
1583
1584
1585
1586
1587
1588
1589
1590
1591
1592
1593
1594
1595
1596
1597
1598
1599
1600
1601
1602
1603
1604
1605
1606
1607
1608
1609
1610
1611
1612
1613
1614
1615
1616
1617
1618
1619
1620
1621
1622
1623
1624
1625
1626
1627
1628
1629
1630
1631
1632
1633
1634
1635
1636
1637
1638
1639
1640
1641
1642
1643
1644
1645
1646
1647
1648
1649
1650
1651
1652
1653
1654
1655
1656
1657
1658
1659
1660
1661
1662
1663
1664
1665
1666
1667
1668
1669
1670
1671
1672
1673
1674
1675
1676
1677
1678
1679
1680
1681
1682
1683
1684
1685
1686
1687
1688
1689
1690
1691
1692
1693
1694
1695
1696
1697
1698
1699
1700
1701
1702
1703
1704
1705
1706
1707
1708
1709
1710
1711
1712
1713
1714
1715
1716
1717
1718
1719
1720
1721
1722
1723
1724
1725
1726
1727
1728
1729
1730
1731
1732
1733
1734
1735
1736
1737
1738
1739
1740
1741
1742
1743
1744
1745
1746
1747
1748
1749
1750
1751
1752
1753
1754
1755
1756
1757
1758
1759
1760
1761
1762
1763
1764
1765
1766
1767
1768
1769
1770
1771
1772
1773
1774
1775
1776
1777
1778
1779
1780
1781
1782
1783
1784
1785
1786
1787
1788
1789
1790
1791
1792
1793
1794
1795
1796
1797
1798
1799
1800
1801
1802
1803
1804
1805
1806
1807
1808
1809
1810
1811
1812
1813
1814
1815
1816
1817
1818
1819
1820
1821
1822
1823
1824
1825
1826
1827
1828
1829
1830
1831
1832
1833
1834
1835
1836
1837
1838
1839
1840
1841
1842
1843
1844
1845
1846
1847
1848
1849
1850
1851
1852
1853
1854
1855
1856
1857
1858
1859
1860
1861
1862
1863
1864
1865
1866
1867
1868
1869
1870
1871
1872
1873
1874
1875
1876
1877
1878
1879
1880
1881
1882
1883
1884
1885
1886
1887
1888
1889
1890
1891
1892
1893
1894
1895
1896
1897
1898
1899
1900
1901
1902
1903
1904
1905
1906
1907
1908
1909
1910
1911
1912
1913
1914
1915
1916
1917
1918
1919
1920
1921
1922
1923
1924
1925
1926
1927
1928
1929
1930
1931
1932
1933
1934
1935
1936
1937
1938
1939
1940
1941
1942
1943
1944
1945
1946
1947
1948
1949
1950
1951
1952
1953
1954
1955
1956
1957
1958
1959
1960
1961
1962
1963
1964
1965
1966
1967
1968
1969
1970
1971
1972
1973
1974
1975
1976
1977
1978
1979
1980
1981
1982
1983
1984
1985
1986
1987
1988
1989
1990
1991
1992
1993
1994
1995
1996
1997
1998
1999
2000
2001
2002
2003
2004
2005
2006
2007
2008
2009
2010
2011
2012
2013
2014
2015
2016
2017
2018
2019
2020
2021
2022
2023
2024
2025
2026
2027
2028
2029
2030
2031
2032
2033
2034
2035
2036
2037
2038
2039
2040
2041
2042
2043
2044
2045
2046
2047
2048
2049
2050
2051
2052
2053
2054
2055
2056
2057
2058
2059
2060
2061
2062
2063
2064
2065
2066
2067
2068
2069
2070
2071
2072
2073
2074
2075
2076
2077
2078
2079
2080
2081
2082
2083
2084
2085
2086
2087
2088
2089
2090
2091
2092
2093
2094
2095
2096
2097
2098
2099
2100
2101
2102
2103
2104
2105
2106
2107
2108
2109
2110
2111
2112
2113
2114
2115
2116
2117
2118
2119
2120
2121
2122
2123
2124
2125
2126
2127
2128
2129
2130
2131
2132
2133
2134
2135
2136
2137
2138
2139
2140
2141
2142
2143
2144
2145
2146
2147
2148
2149
2150
2151
2152
2153
2154
2155
2156
2157
2158
2159
2160
2161
2162
2163
2164
2165
2166
2167
2168
2169
2170
2171
2172
2173
2174
2175
2176
2177
2178
2179
2180
2181
2182
2183
2184
218

- 6 40. A method as defined in either of claims 38 or 39 further comprising:
- 5
- 4 through other branch of the body lumen.
- 3 other branch of the trunk by advancing the other leg extension endoluminally
- 2 similarly placing within and engaging another leg extension with the
- 1 39. A method as defined in claim 38 further comprising:
- 17 extension with the inner surface of the trunk.
- 16 effecting secure engagement of the inserted end of the leg
- 15 branch body lumen and into one of the tubular branch member of the trunk; and
- 14 inserting one end of the leg extension transluminally through a
- 13 providing a radially expandable tubular elongate leg extension;
- 12 the other branches of the bifurcated body lumen;
- 11 the branch tubes being spaced from but being transluminally accessible through
- 10 securely placing the trunk in one branch of the body vessel, with
- 9 tubular branch members;
- 8 providing a tubular trunk having a main tubular body and a pair of
- 7 comprising:
- 6 38. A method of placing a bifurcated graft in a bifurcated body lumen
- 5
- 4 open ends of the branch tubes.
- 3 tubes and being configured to provide a radiographic image of the location of the
- 2 a radiopaque member associated with the lower ends of the branch
- 1 37. An implant as defined in claim 35 further comprising:
- 4 at least two struts connecting the anchor and the stent.
- 3 maintaining the lower ends of the branch tubes in an open configuration;
- 2 anchor at the upper end of the trunk and a stent at the lower end of the trunk for
- 1 36. An implant as defined in claim 35 wherein the frame comprises an

- 4
3
2
1
6
5
4
3
2
1
12
11
10
9
8
7
6
5
4
3
2
1
8
7
- end of the trunk.
instrumentalities crossing over each other at a location spaced from the lower
advanced through each of the branches of the bifurcated body lumen, with the
43. A method as defined in claim 42 wherein instrumentality is
engagement with the aligned tubular branch member of the trunk.
through said body branch may be advanced in general alignment and into
bifurcated body lumen whereby subsequently placed instrumentalities inserted
general alignment with the direction extending from one of the branches of the
orienting the tubular trunk so that its open lower end is disposed in
42. A method as defined in claim 38 further comprising:
leg to engage the inner surface of the trunk in surface-to-surface engagement.
releasing the overlapped portion of the leg to enable that end of the
overlapping relation to the trunk; and
advancing a tubular leg into one of the branch tubes of the trunk in
lumen end of the trunk into secure engagement with the supportive tissue;
releasing the trunk while effecting the expansion of the single
the other end is spaced from the bifurcate region of the body lumen;
that its upper end is aligned with supportive tissue in one of the body lumens and
advancing the delivery device endoluminally to locate the trunk so
contracting the trunk within a delivery device;
step of placing the trunk comprises:
41. A method as defined in either one of claims 38 or 39 wherein the
securing the other end of each of the leg extensions to supportive
tissue in the other branches of the body lumen.

1 44. An apparatus for delivering and deploying an expandable implant
2 within a blood vessel comprising:
3 a tubular sheath for maintaining the implant in a radial contracted
4 configuration, the sheath having a proximal end and a distal end and being open
5 at its distal end and axially movable relative to the implant;
6 a gripping device disposed within and longitudinally of the sheath,
7 the gripping device being constructed to releasably grip the trailing end of a
8 tubular implant;

9 the gripping device further comprising a cup having a distally facing
10 open end adapted to receive the trailing end of the tubular implant and a gripping
11 member movably mounted with respect to the cup between a gripping position in
12 which the member is withdrawn into the cup to define an annular space between
13 its periphery and the interior of the cup and a release position in which the
14 member is disposed out of the cup;
15 the annular space being sufficiently narrow to enable the trailing
16 end of the tubular member to be securely gripped between the member and the
17 cup when the member and cup are in the gripping position.

FIG. 1

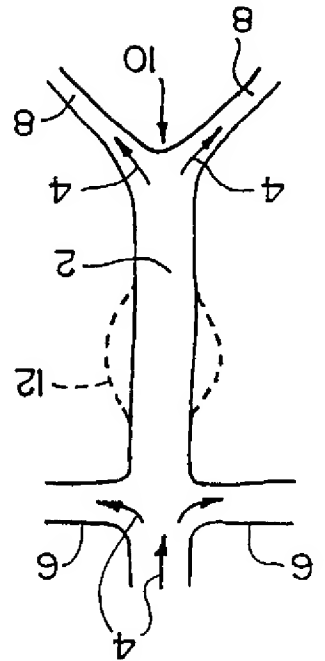
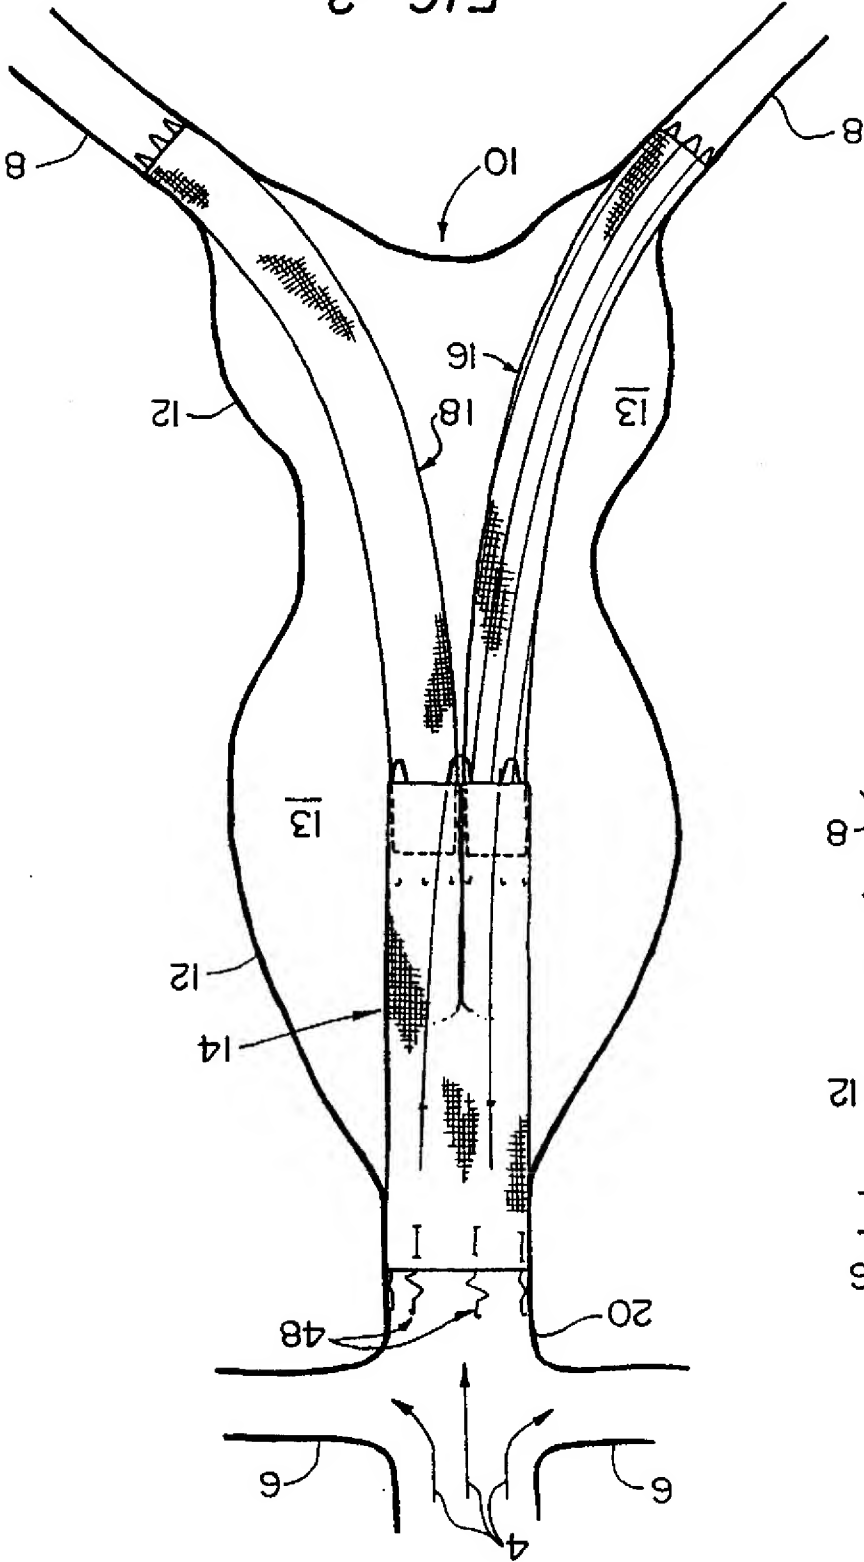


FIG. 2



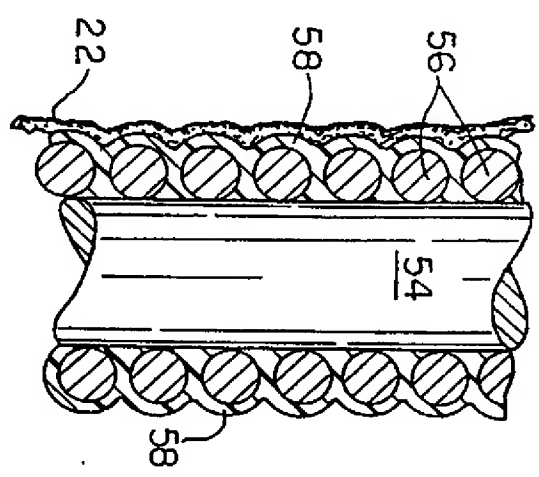


FIG. 7

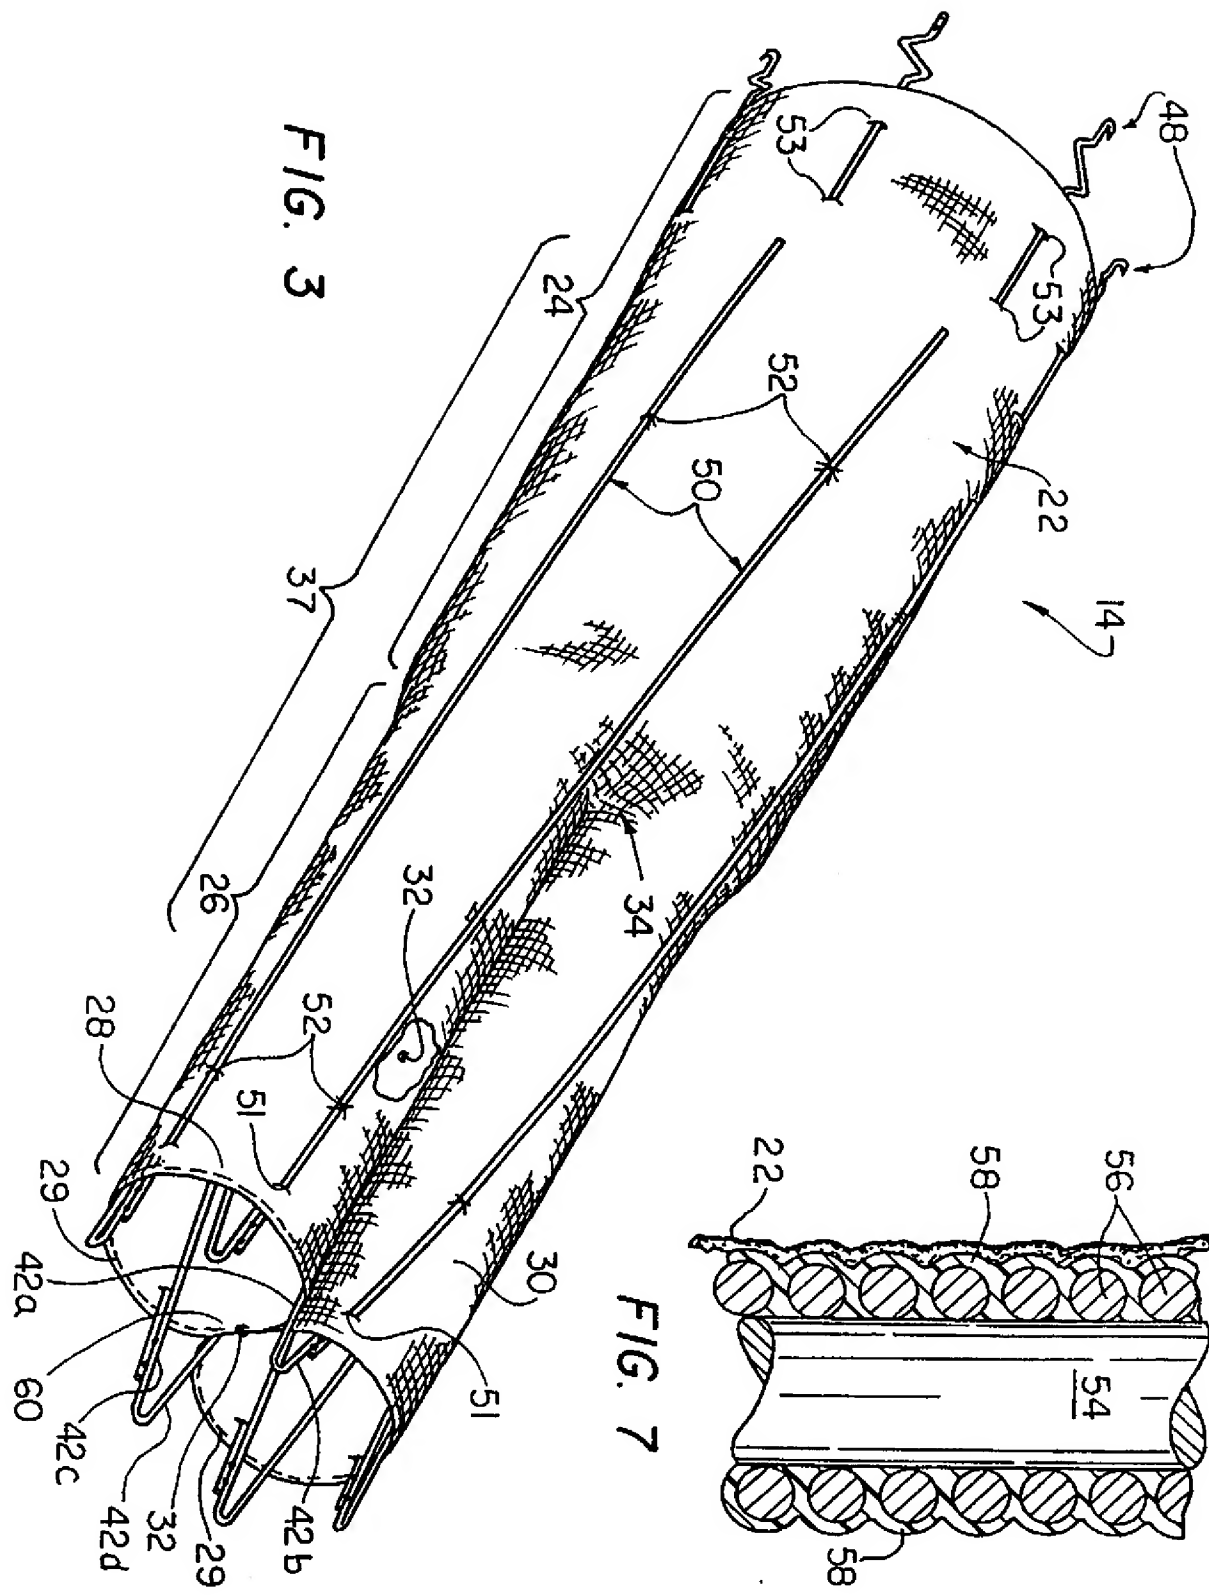
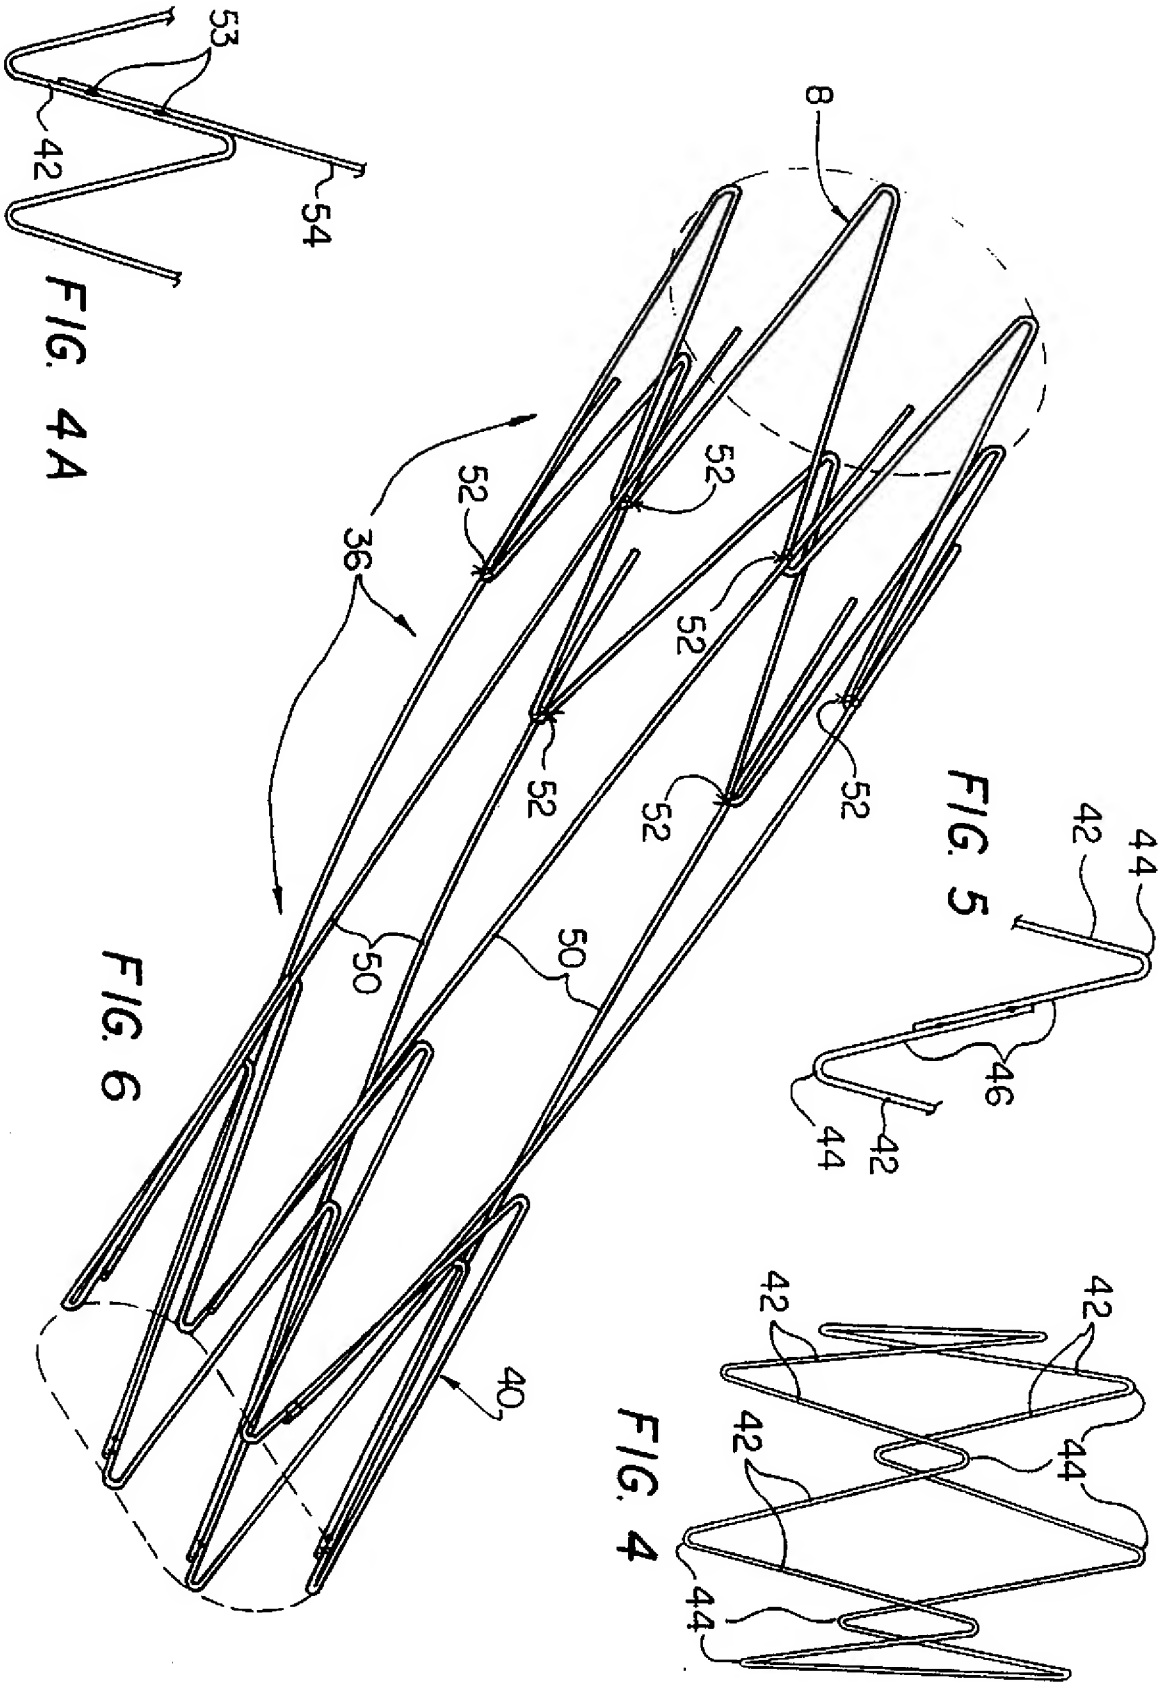


FIG. 3



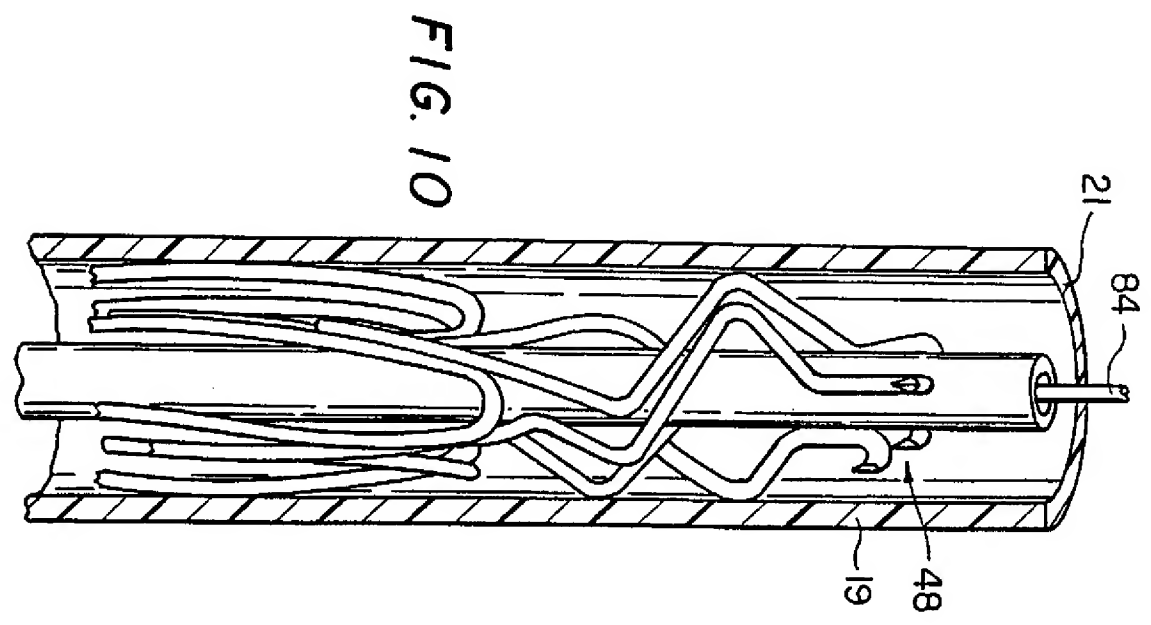
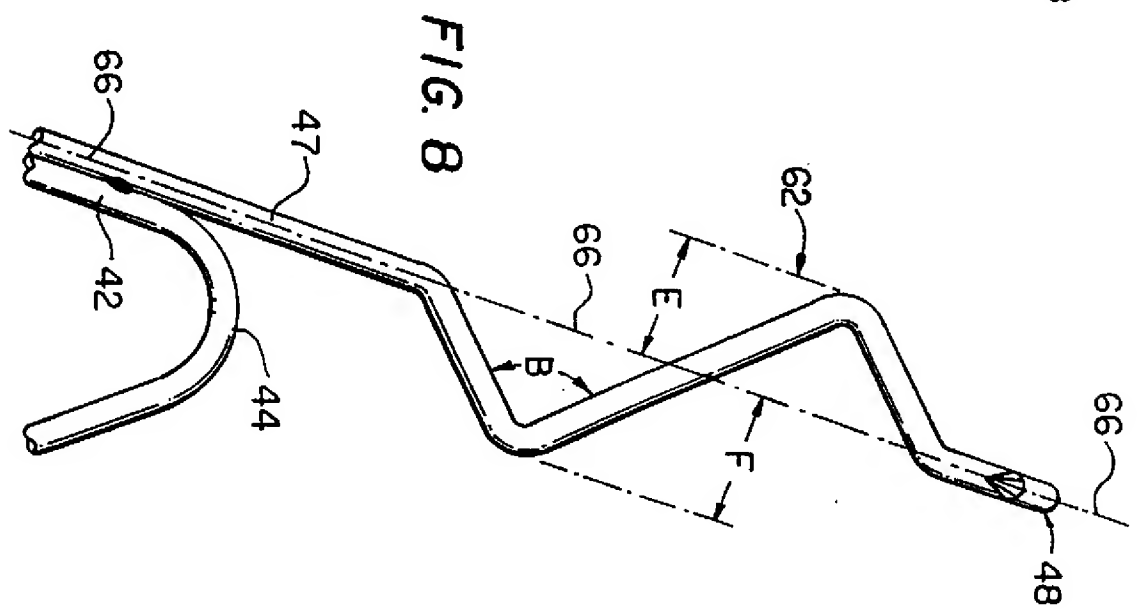
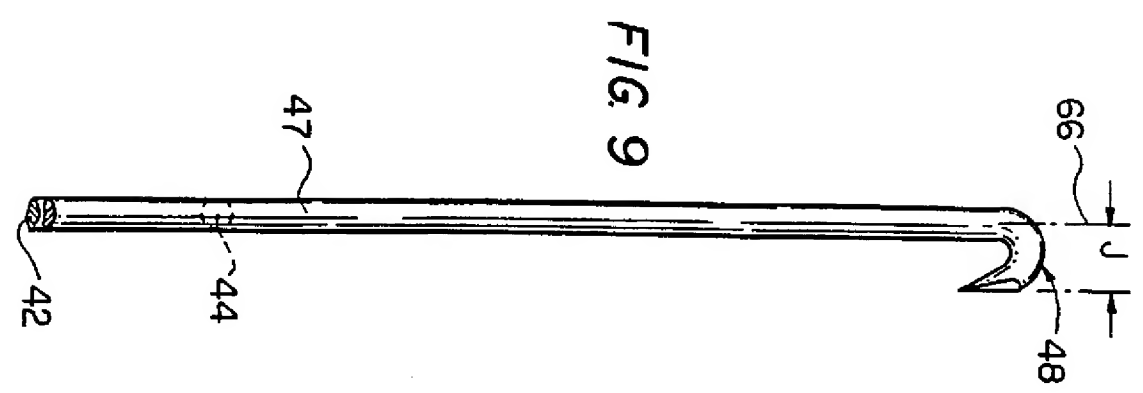


FIG. 13

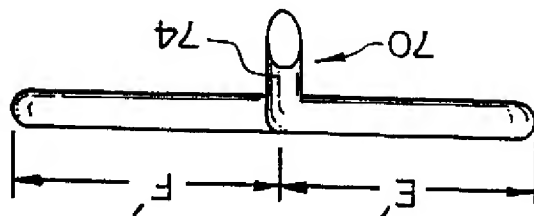


FIG. 14

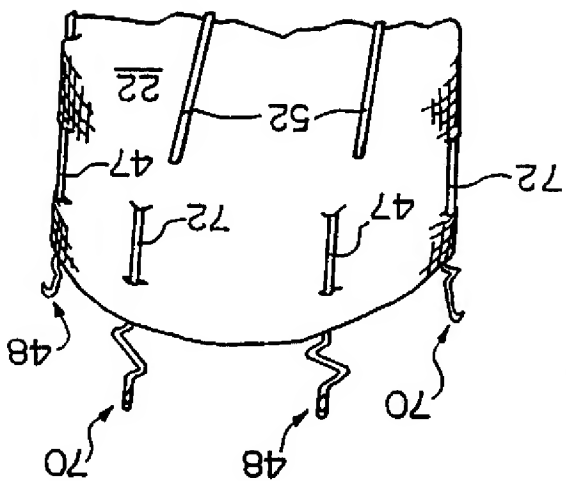


FIG. 11

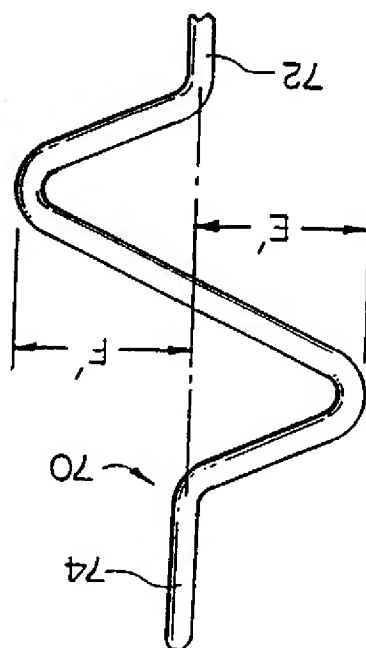


FIG. 12

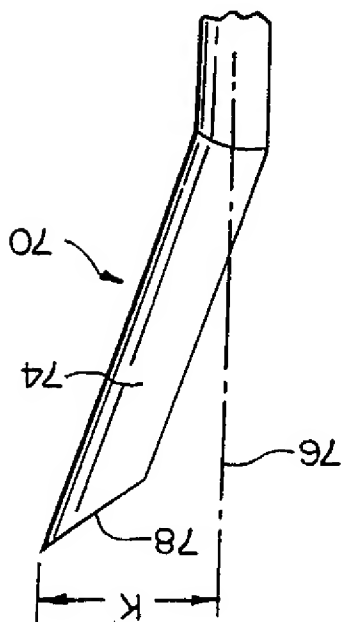


FIG. 16

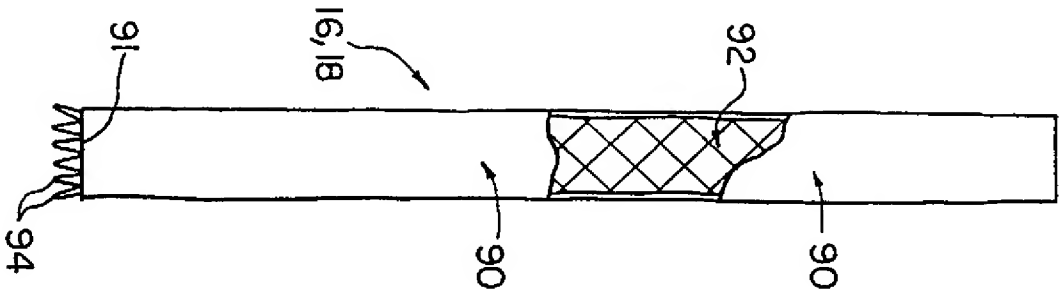


FIG. 15

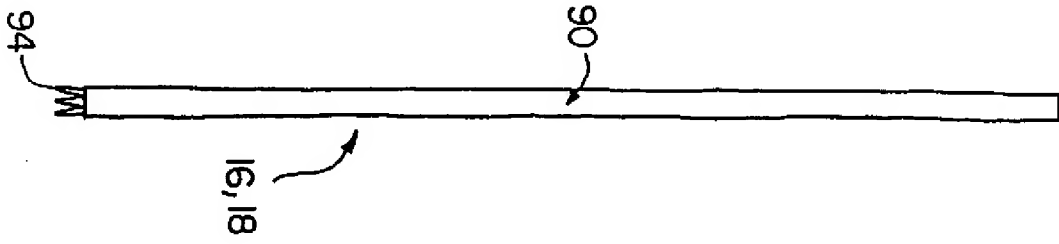


FIG. 17

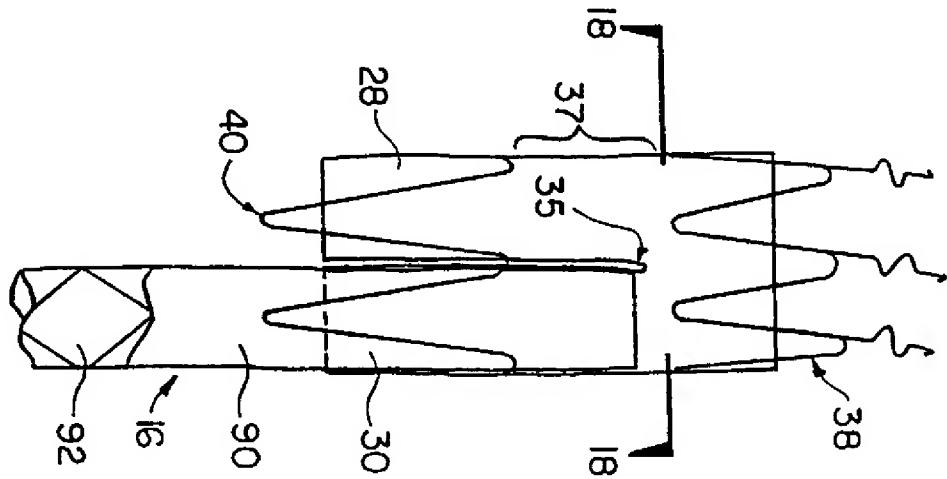
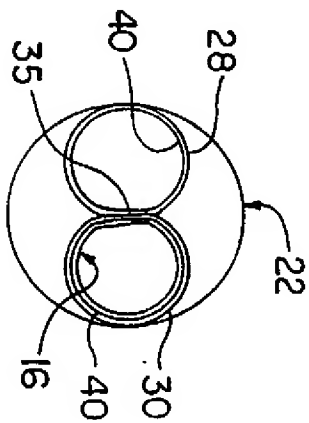


FIG. 18



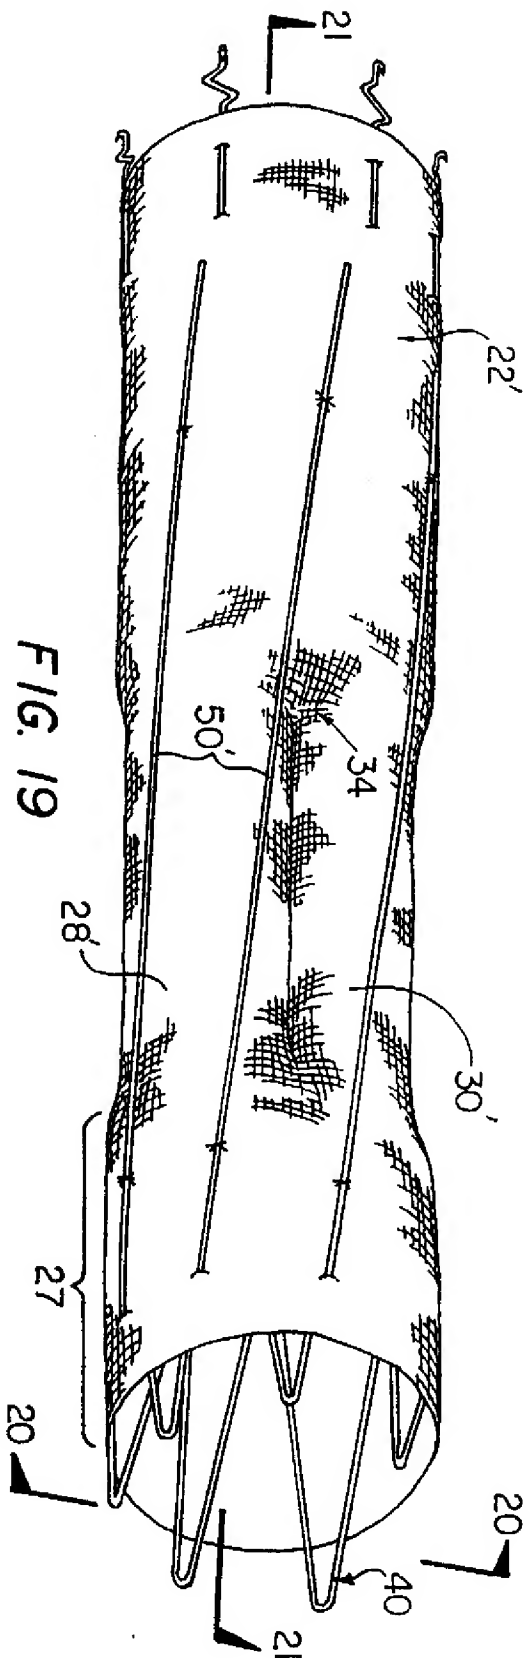


FIG. 19

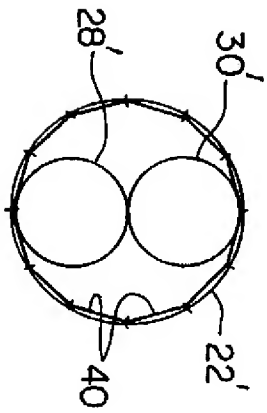


FIG. 20

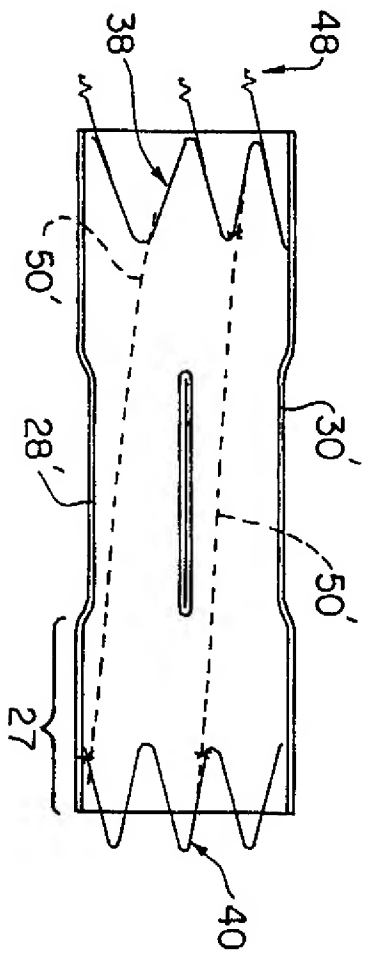


FIG. 21

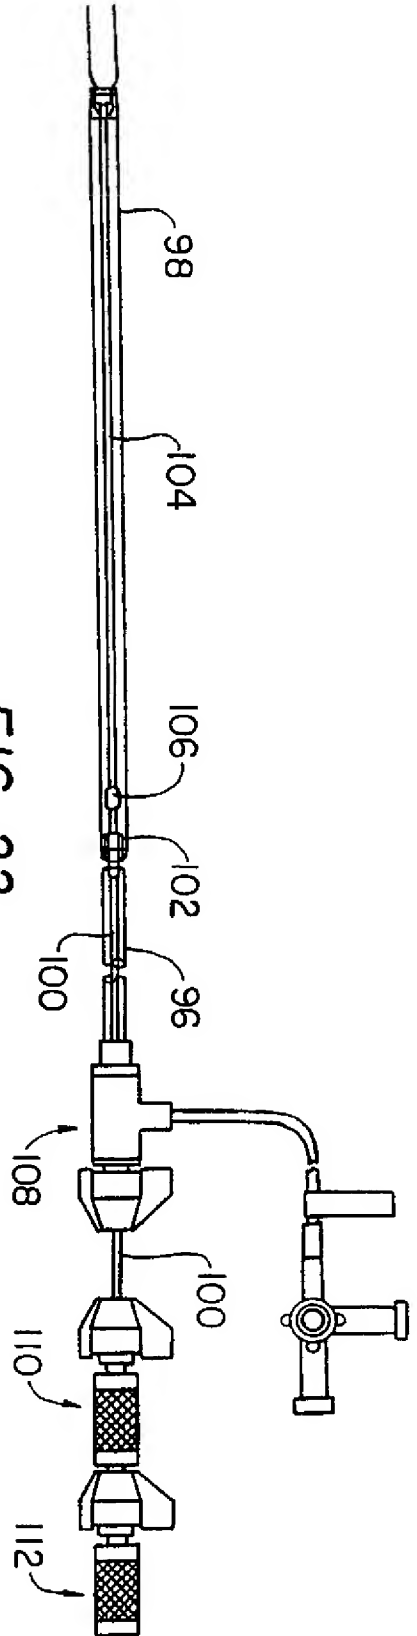


FIG. 22

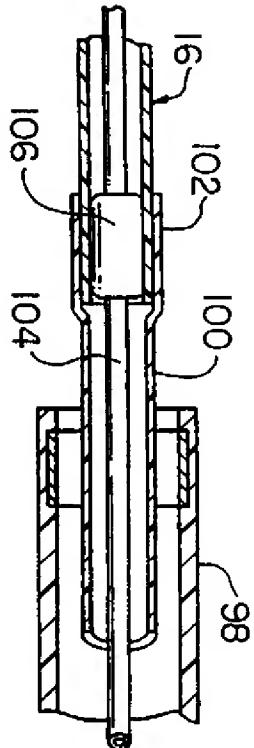


FIG. 23

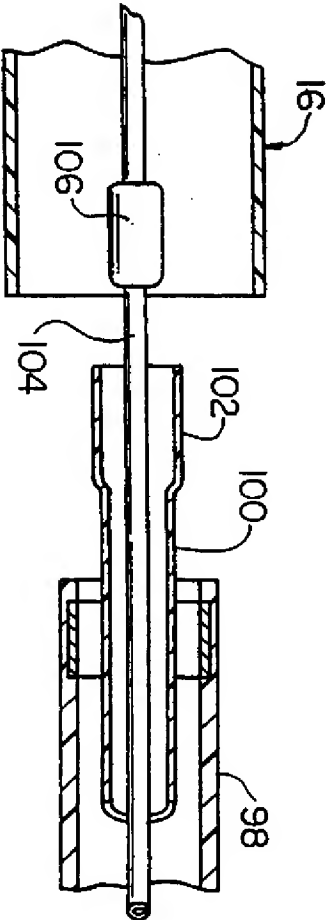


FIG. 24

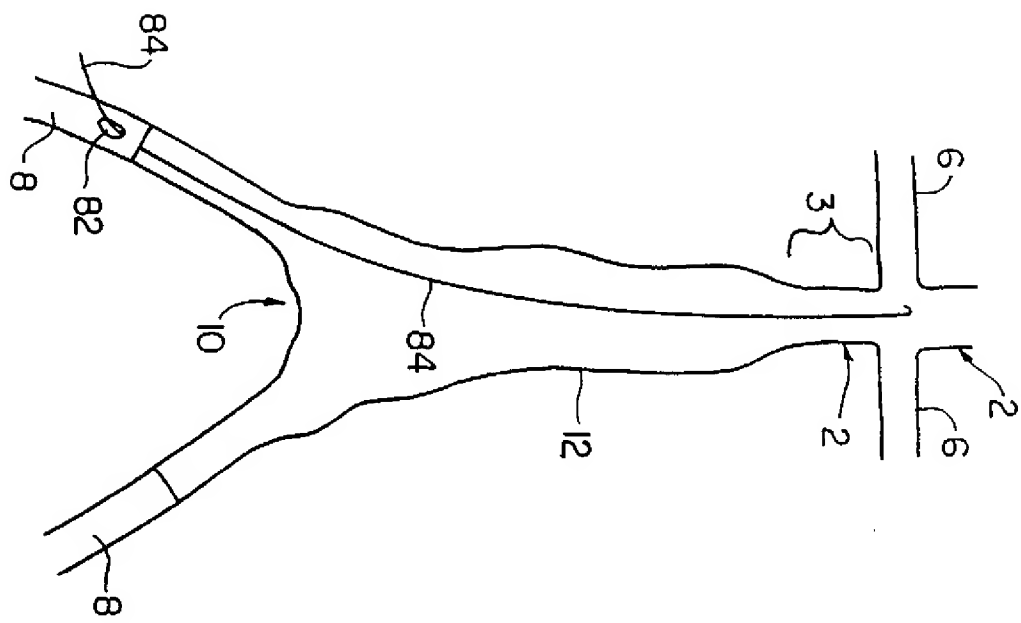


FIG. 25A

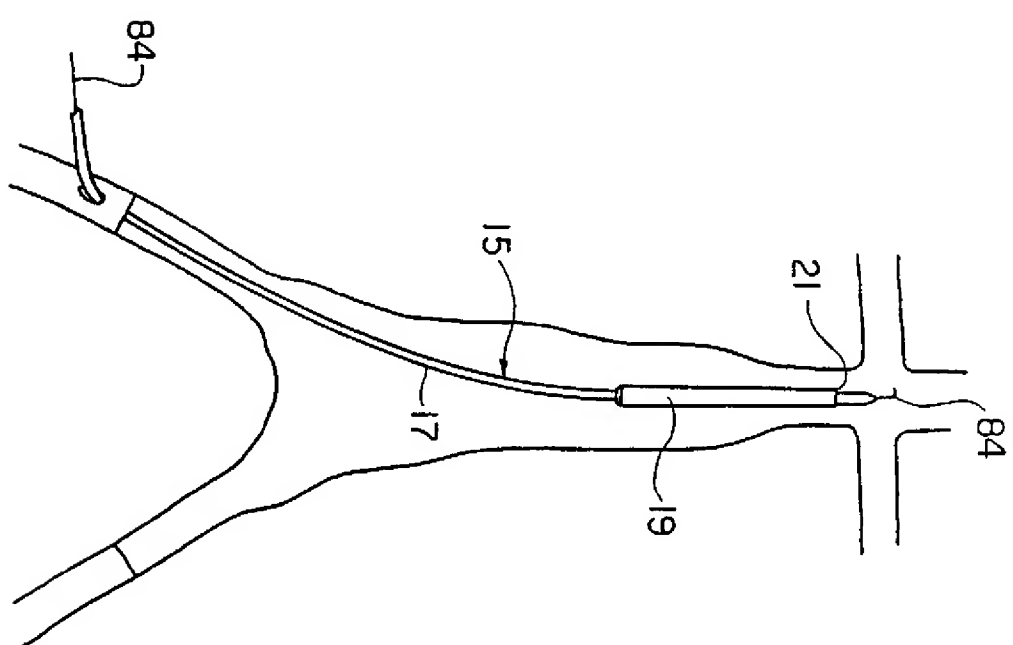


FIG. 25B

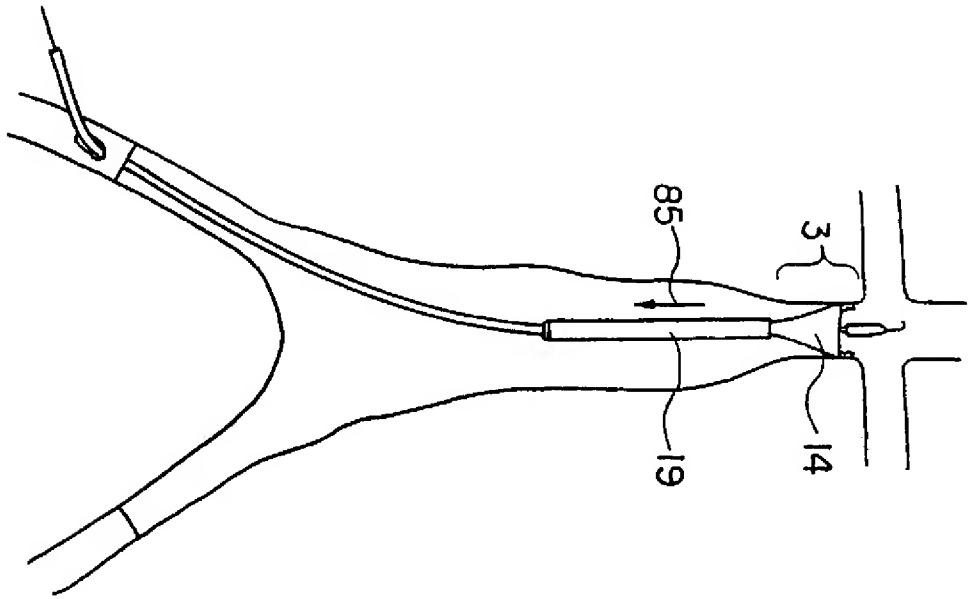


FIG. 25C

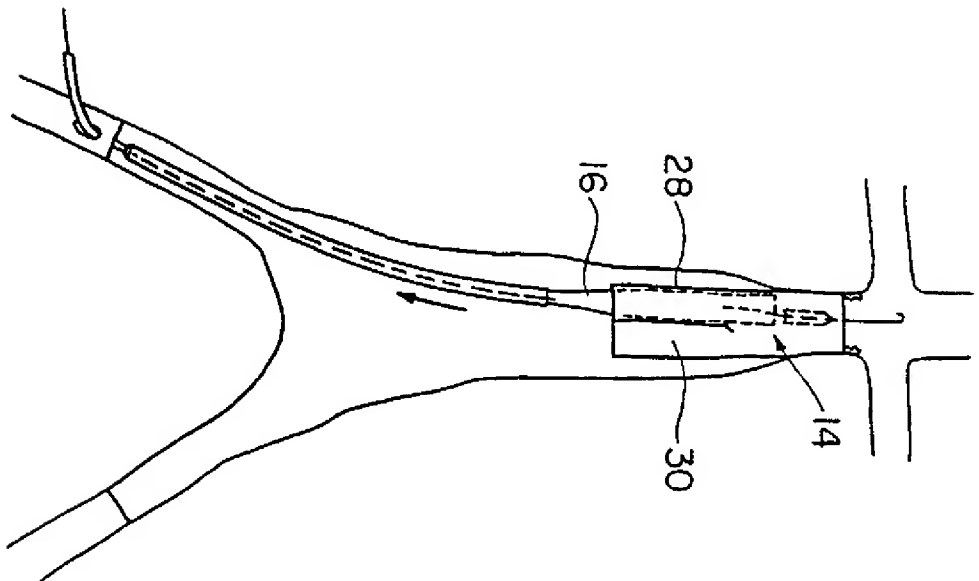


FIG. 25D

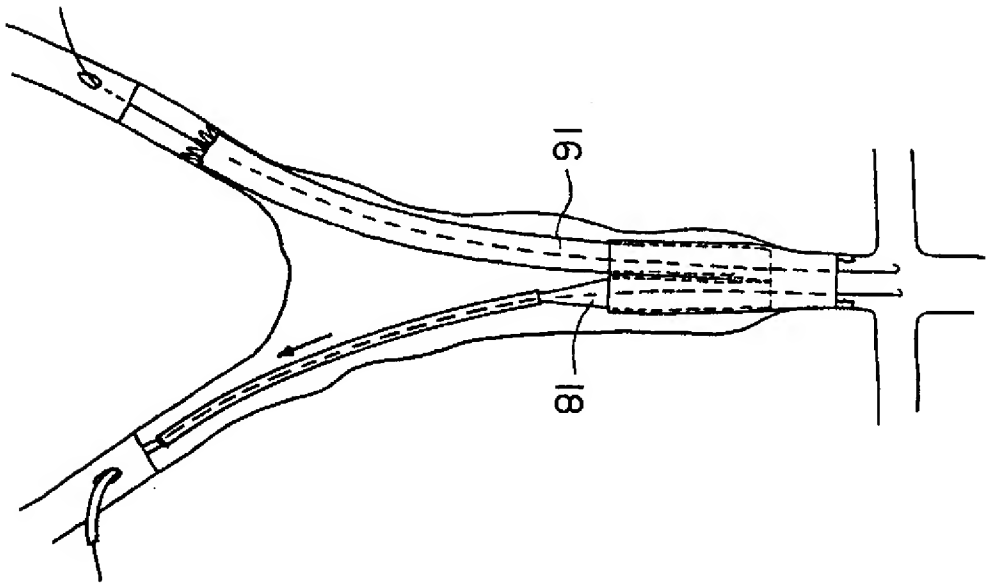


FIG. 25E

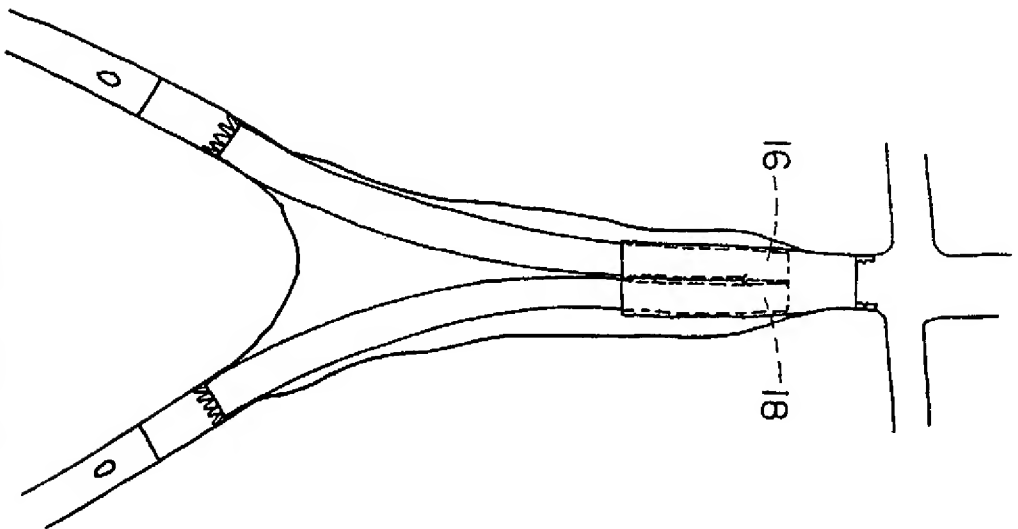


FIG. 25F

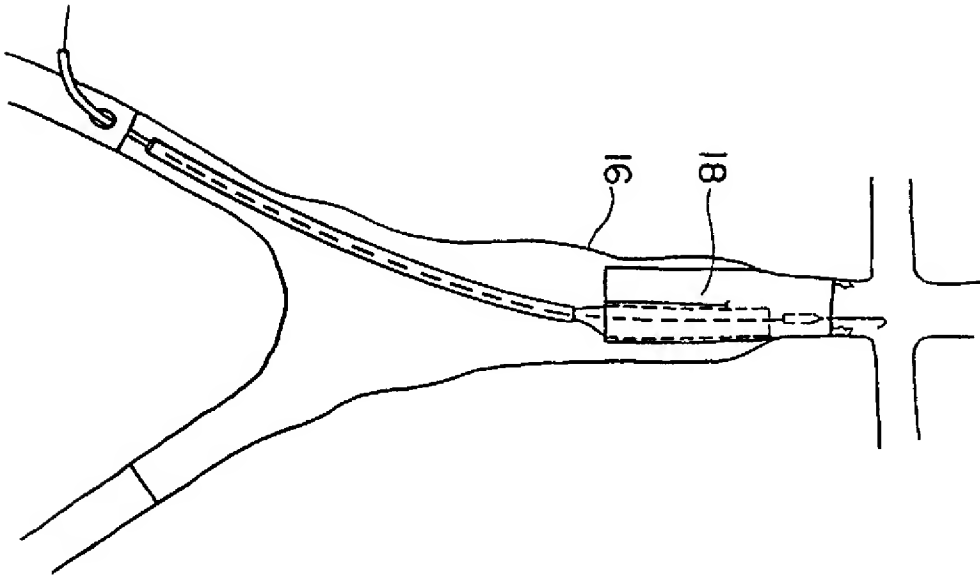


FIG. 26D

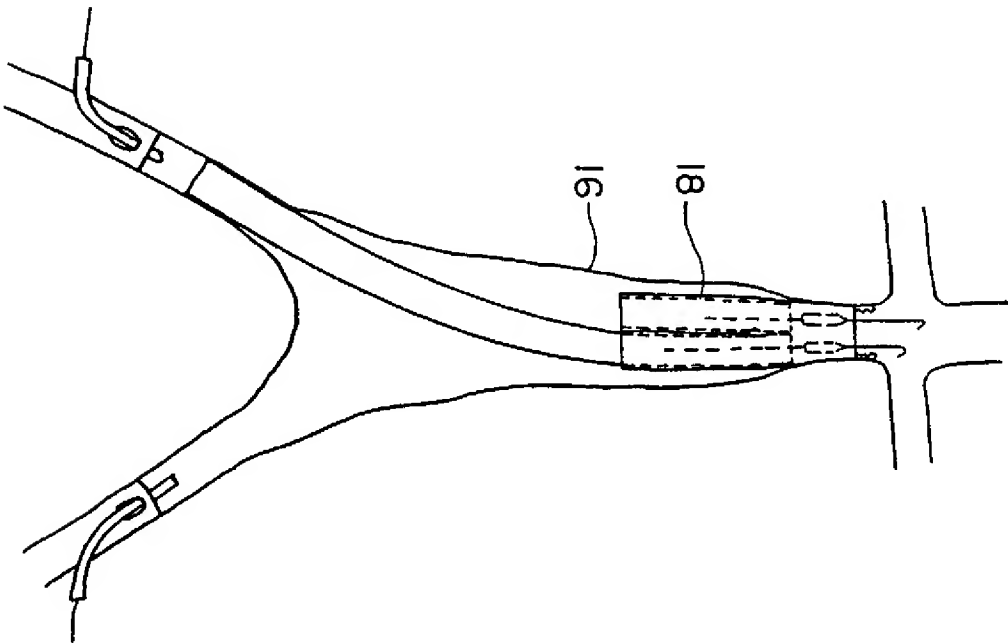


FIG. 26E

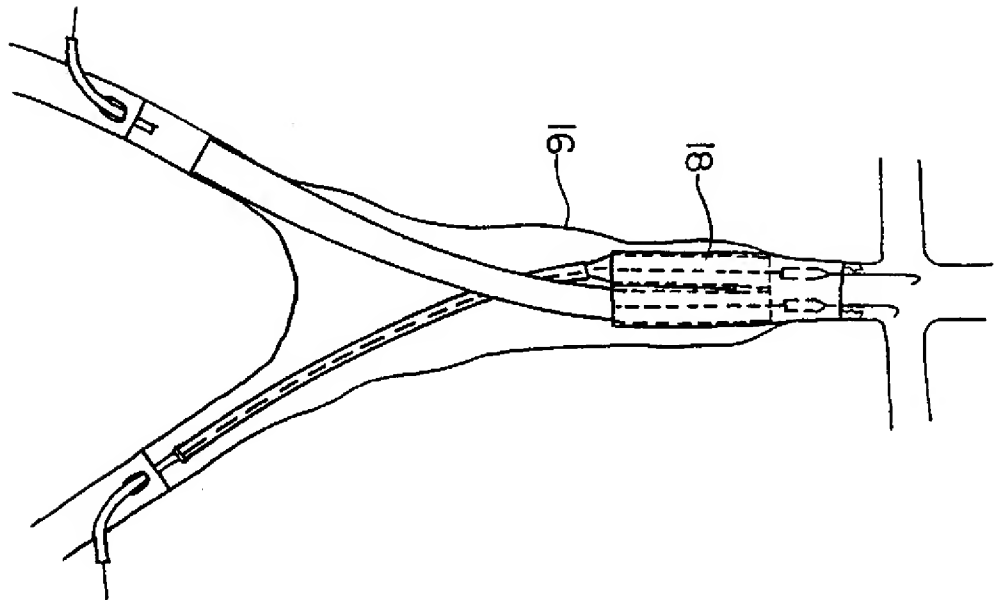


FIG. 26 F



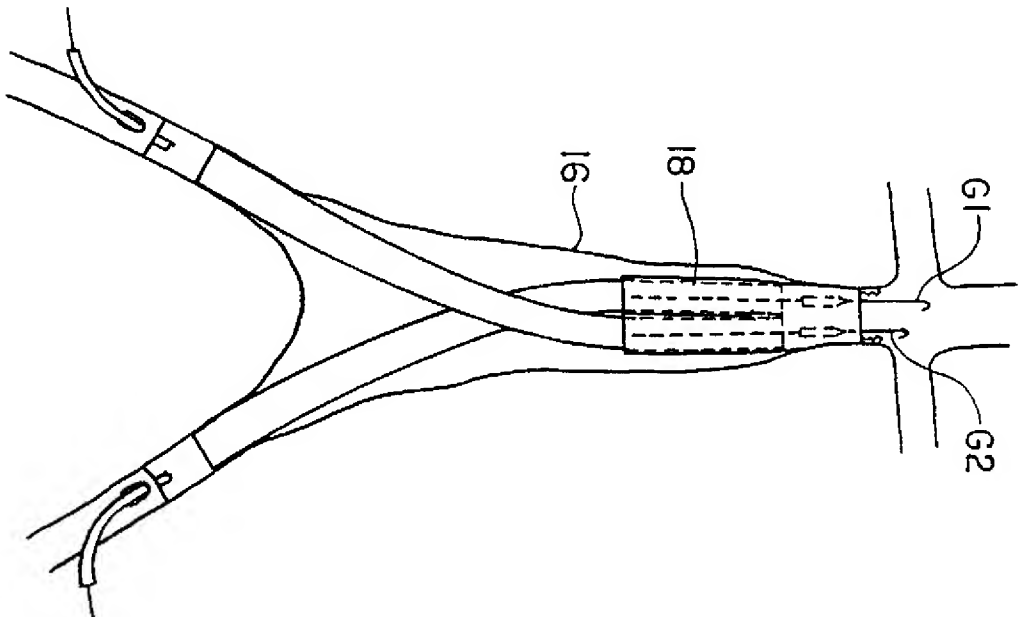


FIG. 26 G

FIG. 27

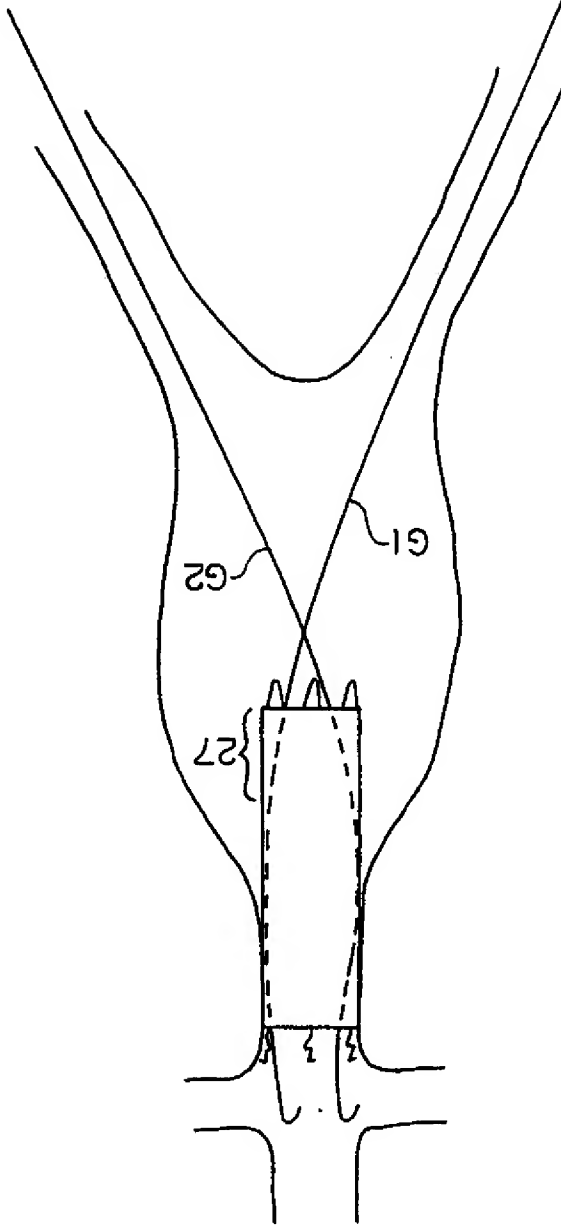

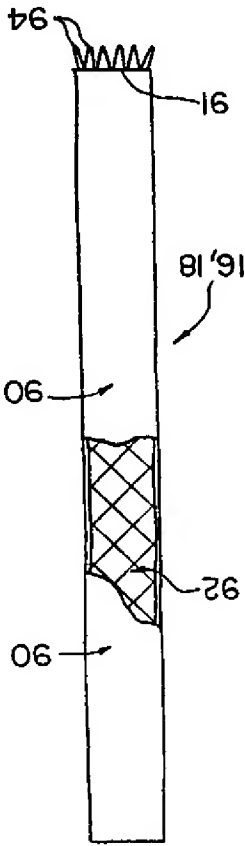

(51) International Patent Classification ⁶ : A61F 2/06		A3	(11) International Publication Number: WO 98/23242	(43) International Publication Date: 4 June 1998 (04.06.98)
(21) International Application Number: PCT/US97/21211			(81) Designated States: AU, CA, JP, European patent (AT, BE, CH, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE).	Published With international search report Before the expiration of the time limit for amending the claims and to be republished in the event of the receipt of amendments. (88) Date of publication of the international search report: 13 August 1998 (13.08.98)
(30) Priority Data: 08/756,061 25 November 1996 (25.11.96) US		(71) Applicant: C.R. BARD, INC. [US/US]; 730 Central Avenue, Murray Hill, NJ 07974 (US).		
(22) International Filing Date: 13 November 1997 (13.11.97)		(72) Inventors: ROBINSON, Timothy; 11 Snow Lane, Sandown, NH 03873 (US). WEISER, Michael, F.; 516 Martins Pond Road, Groton, MA 01450 (US). KUJAWSKI, Dennis; 25 Parker Road, Brookline, NH 03033 (US). DWYER, Clifford, J.; 9 Moore Street, Wilmington, MA 01887 (US).		
(74) Agent: BOOKSTEIN, Arthur; One Beacon Street, Boston, MA 02108 (US).		(54) Title: MODULAR ENDOPROSTHESIS		
(57) Abstract <p>An endoprosthetic implant is formed from a plurality of separate individual components that are inserted sequentially and transminally into a bifurcated vascular region with each component being deployed in sequence by a sequence of catheter-like deployment devices. The separate components are placed relative to each other to define a bifurcated sheath for maintaining the radially expandable tubular implant in a contracted configuration and a gripping device including a cup and a gripping member that cooperate to define an annular space by which the trailing end of the implant can be securely held by the deployment device during positioning of the device.</p>				

AL	Albania	ES	Spain	LS	Lesotho	SI	Slovenia
AM	Armenia	FI	Finland	LT	Lithuania	SK	Slovakia
AT	Austria	FR	France	LU	Luxembourg	SN	Senegal
AU	Australia	GA	Gabon	LV	Latvia	SZ	Swaziland
AZ	Azerbaijan	GB	United Kingdom	MC	Monaco	TD	Chad
BA	Bosnia and Herzegovina	GE	Georgia	MD	Republic of Moldova	TG	Togo
BB	Barbados	GH	Ghana	MG	Madagascar	TJ	Tajikistan
BE	Belgium	GN	Guinea	MK	The former Yugoslav	TM	Turkmenistan
BF	Burkina Faso	GR	Greece	ML	Republic of Macedonia	TR	Turkey
BG	Bulgaria	HU	Hungary	MN	Mongolia	TT	Trinidad and Tobago
BJ	Benin	IE	Ireland	MR	Mauritania	UA	Ukraine
BR	Brazil	IL	Israel	MW	Malawi	UG	Uganda
BY	Belarus	IS	Iceland	MX	Mexico	US	United States of America
CA	Canada	IT	Italy	NE	Niger	VN	Viet Nam
CF	Central African Republic	JP	Japan	NL	Netherlands	YU	Yugoslavia
CG	Congo	KE	Kenya	NO	Norway	ZW	Zimbabwe
CH	Switzerland	KG	Kyrgyzstan	NZ	New Zealand		
CI	Cote d'Ivoire	KP	Democratic People's				
CN	China	KR	Republic of Korea				
CU	Cuba	KZ	Kazakhstan				
CZ	Czech Republic	LC	Saint Lucia				
DE	Germany	LI	Liechtenstein				
DK	Denmark	LK	Sri Lanka				
EE	Estonia	LR	Liberia				
				SC	Singapore		
				SE	Sweden		
				SD	Sudan		
				RU	Russian Federation		
				RO	Romania		
				PT	Portugal		
				PL	Poland		
				NZ	New Zealand		
				NO	Norway		
				NL	Netherlands		
				MX	Mexico		
				MW	Malawi		
				MR	Mauritania		
				MN	Mongolia		
				ML	Mali		
				MG	Madagascar		
				MD	Republic of Moldova		
				MC	Monaco		
				LV	Latvia		
				LU	Luxembourg		
				LT	Lithuania		
				LS	Lesotho		

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

FOR THE PURPOSES OF INFORMATION ONLY

INTERNATIONAL SEARCH REPORT

Internal, All Application No
PCT/US 97/21211

A. CLASSIFICATION OF SUBJECT MATTER
IPC 6 A61F2/06

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)
IPC 6 A61F

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
------------	--	-----------------------

X	WO 96 24308 A (COOK INCORPORATED) 15 August 1996 see the whole document	1-3, 6-8, 15-23, 9, 11-13, 25-28, 30, 31, 33-37
Y	FR 2 722 678 A (B BRAUN CELSA) 26 January 1996 see the whole document	9, 11-13, 25-28, 30, 31, 33-37
Y	WO 96 23455 A (BOSTON SCIENTIFIC CORPORATION) 8 August 1996 see abstract; figures	1

☐ Further documents are listed in the continuation of box C.

☒ Patent family members are listed in annex.

* Special categories of cited documents:

- "A" document defining the general state of the art which is not considered to be of particular relevance
- "E" earlier document but published on or after the international filing date
- "L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another document or other special reason (as specified)
- "O" document referring to an oral disclosure, use, exhibition or other means
- "P" document published prior to the international filing date but later than the priority date claimed
- "g" document member of the same patent family

Date of the actual completion of the international search	23 March 1998
Date of mailing of the international search report	25.06.98

Name and mailing address of the ISA European Patent Office, P.B. 5818 Patentkan 2 NL - 2280 HV Rijswijk Tel. (+31-70) 340-2040, Tx. 31 651 epo nl Fax: (+31-70) 340-3016	Authorized officer Smith, C
--	--------------------------------

INTERNATIONAL SEARCH REPORT

Int'l application No.

PCT/US 97/21211

Box I Observations where certain claims were found unsearchable (Continuation of Item 1 of first sheet)

This International Search Report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons:

1. ☒ Claims Nos.: 38-43
because they relate to subject matter not required to be searched by this Authority, namely:
Please see Rule 39.1(iv) PCT - Method for treatment of the human or animal body by surgery.
2. ☐ Claims Nos.:
because they relate to parts of the International Search can be carried out, specifically:
an extent that no meaningful International Search can be carried out, specifically:
3. ☐ Claims Nos.:
because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a).

Box II Observations where unity of invention is lacking (Continuation of Item 2 of first sheet)

This International Searching Authority found multiple inventions in this international application, as follows:

See Annex

1. ☐ As all required additional search fees were timely paid by the applicant, this International Search Report covers all searchable claims.

2. ☐ As all searchable claims could be searched without effort justifying an additional fee, this Authority did not invite payment of any additional fee.

3. ☐ As only some of the required additional search fees were timely paid by the applicant, this International Search Report covers only those claims for which fees were paid, specifically claims Nos.:

4. ☒ No required additional search fees were timely paid by the applicant. Consequently, this International Search Report is restricted to the invention first mentioned in the claims; it is covered by claims Nos.:

1-37

Remark on Protest

- ☐ The additional search fees were accompanied by the applicant's protest.
- ☐ No protest accompanied the payment of additional search fees.

MULTIPLE INVENTIONS

1. Claims: 1-37
A modular endoluminally placeable prosthetic implant.
2. Claim: 44
An apparatus for delivering and deploying an expandable implant within a blood vessel.

INTERNATIONAL SEARCH REPORT

Information on patent family members

International Application No
PCT/US 97/21211

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
---	---------------------	----------------------------	---------------------

WO 9624308 A	15-08-96	US 5693084 A	02-12-97
		AU 687304 B	19-02-98
		AU 4972296 A	27-08-96
		CA 2212286 A	15-08-96
		EP 0808140 A	26-11-97
		US 5720776 A	24-02-98

FR 2722678 A	26-01-96	NONE	
--------------	----------	------	--

WO 9623455 A	08-08-96	US 5755770 A	26-05-98
		CA 2209377 A	08-08-96
		EP 0806917 A	19-11-97